

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071421\
Data File : PD064257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 11:14
Operator : AR\AJ
Sample : M2996-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
C0AT5

Manual Integrations
APPROVED

mohammad
7/15/2021 8:29:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 05:39:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

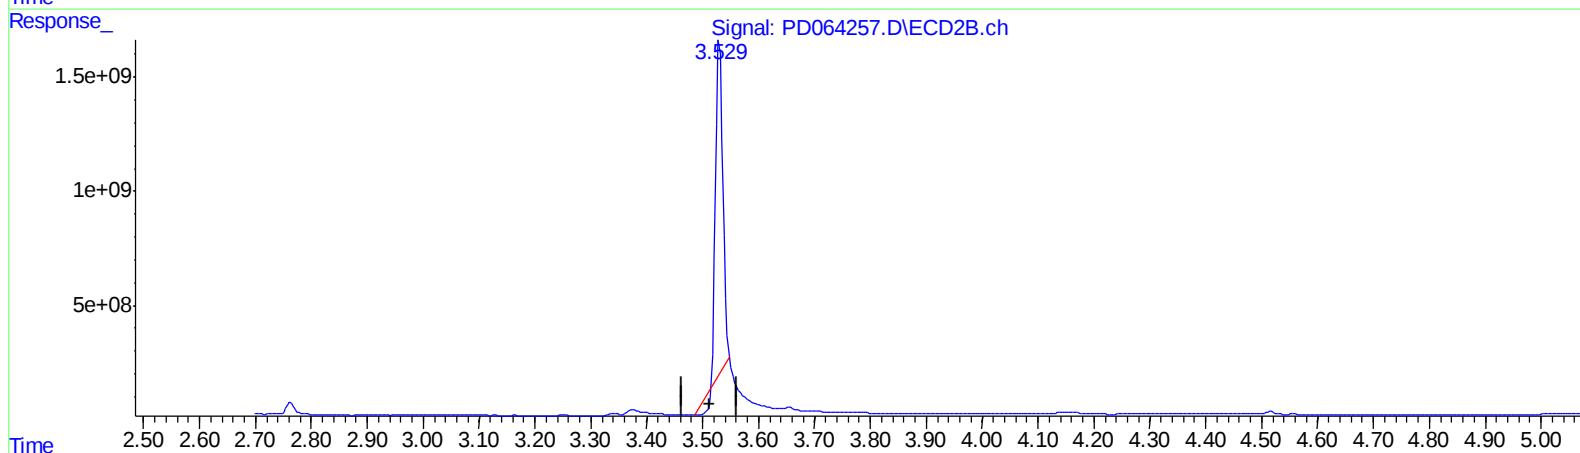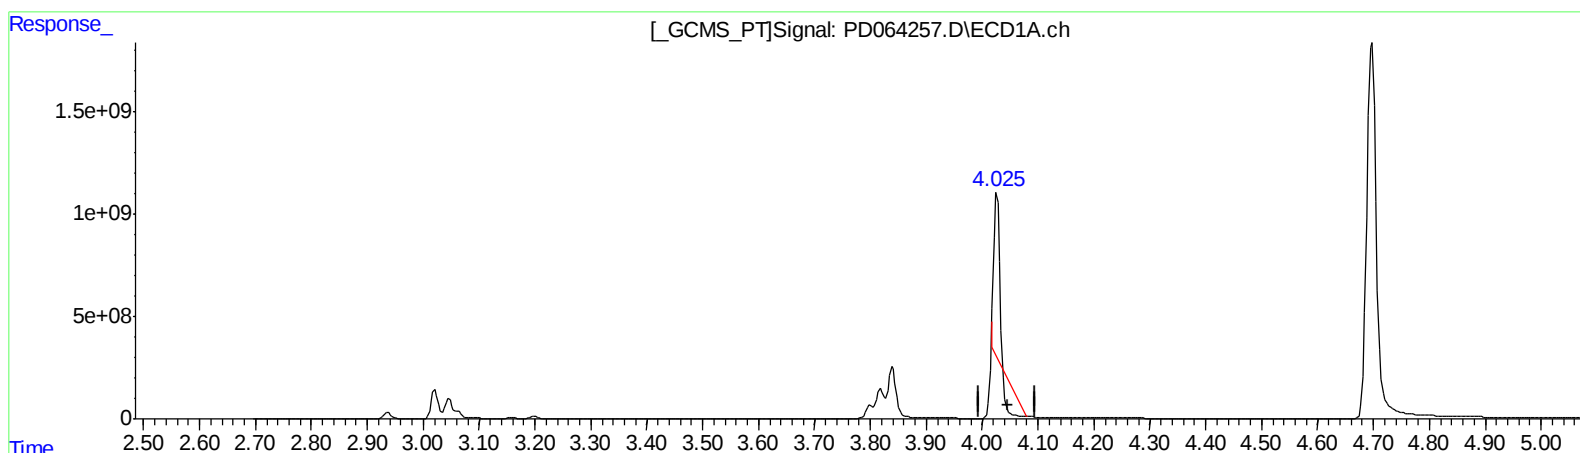

QEdit

(1) Tetrachloro-m-xylene (SA)

4.027min 2396.148 ng/ml

response 3205986097

(1) Tetrachloro-m-xylene #2 (SA)

3.530min 1269.143 ng/ml

response 12680431956

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071421\
Data File : PD064257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 11:14
Operator : AR\AJ
Sample : M2996-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AT5

Manual Integrations
APPROVED

mohammad
7/15/2021 8:29:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 05:39:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.025	3.529	10790.5E6	18496.1E6	8064.816m	1851.212m#
27) SA Decachlor...	9.208	8.254	28267112	108.9E6	26.357	20.840

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

5 AJ
07/19/21