

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
 Data File : PD070901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2022 02:52
 Operator : AR\AJ
 Sample : N3600-02MS
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN4MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/14/2022
 Supervised By : Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 07:39:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.123	38902740	396.0E6	16.168	16.874
27)	SA Decachlor...	8.244	9.319	79157221	288.9E6	31.178	31.285
Target Compounds							
2)	A alpha-BHC	3.914	4.528	157.4E6	1232.6E6	41.956	40.838
3)	MA gamma-BHC...	4.198	4.822	149.1E6	1073.1E6	40.953	41.466
4)	MA Heptachlor	4.499	5.338	145.5E6	762.6E6	41.751	38.052
5)	MB Aldrin	4.747	5.651	149.8E6	661.3E6	41.447	37.998
6)	B beta-BHC	4.448	4.996	62041454	433.7E6	39.600	32.431m
7)	B delta-BHC	4.653	5.222	155.0E6	904.5E6	44.495	39.878
8)	B Heptachlo...	5.192	6.046	137.7E6	557.9E6	41.345	37.571
9)	A Endosulfan I	5.532	6.410	127.8E6	500.2E6	42.409	37.718
10)	B trans-Chl...	5.419	6.282	142.7E6	562.2E6	41.008	37.338
11)	B cis-Chlor...	5.478	6.356	139.3E6	530.2E6	40.759	36.709
12)	B 4,4'-DDE	5.644	6.510	271.1E6	1046.5E6	84.254	76.303
13)	MA Dieldrin	5.776	6.672	294.9E6	1091.7E6	88.063	78.838
14)	MA Endrin	6.035	6.895	254.9E6	878.8E6	91.934	84.165
15)	B Endosulfa...	6.308	7.109	238.2E6	880.5E6	86.840	76.440
16)	A 4,4'-DDD	6.162	7.010	215.1E6	882.9E6	82.576	80.728
17)	MA 4,4'-DDT	6.403	7.312	239.1E6	937.6E6	89.373	83.781
18)	B Endrin al...	6.478	7.234	166.9E6	665.9E6	72.839	68.488
19)	B Endosulfa...	6.691	7.459	226.5E6	835.8E6	80.871	73.726
20)	A Methoxychlor	6.954	7.771	589.6E6	2063.2E6	426.383	394.340
21)	B Endrin ke...	7.185	7.940	266.4E6	971.8E6	85.941	78.698

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
Data File : PD070901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2022 02:52
Operator : AR\AJ
Sample : N3600-02MS
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 07:39:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

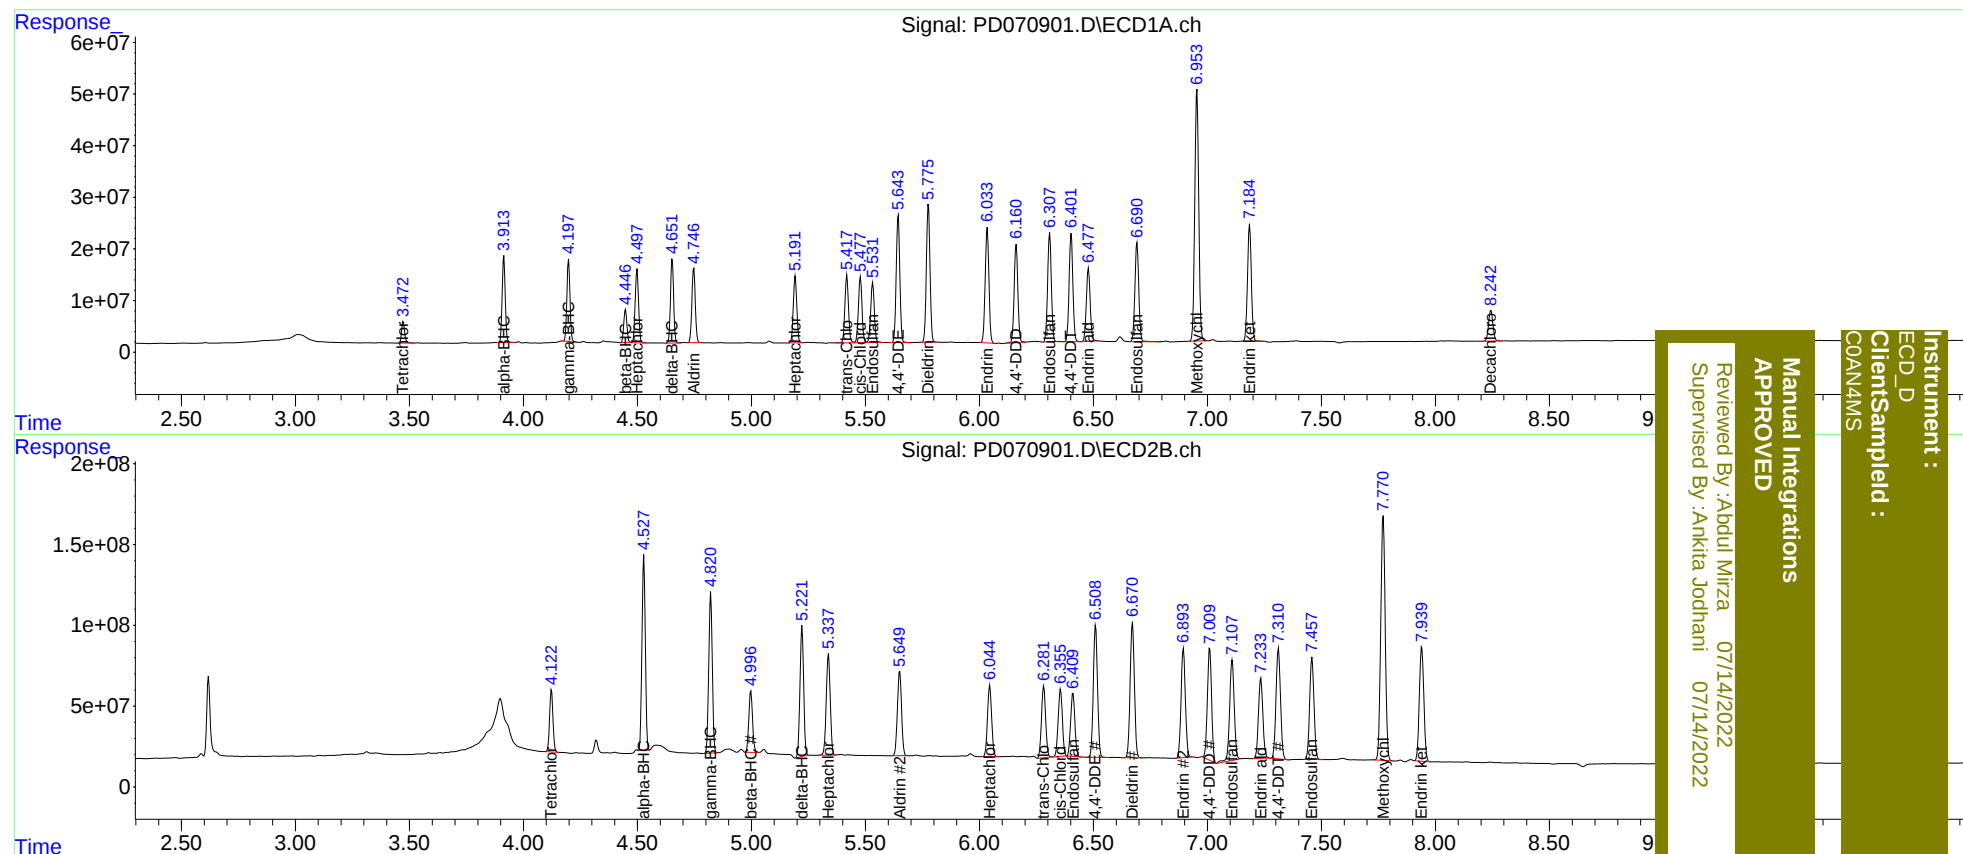

Instrument :
ECD_D
ClientSampled :
COAN4MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/14/2022
Supervised By: Ankita Jodhani 07/14/2022