

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD071422\  
 Data File : PD070902.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Jul 2022 03:07  
 Operator : AR\AJ  
 Sample : N3600-03MSD  
 Misc :  
 ALS Vial : 41 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 C0AN4MSD

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 07/14/2022  
 Supervised By : Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 14 07:39:45 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD071422CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jul 14 05:14:58 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|---------|
| -----                       |                 |       |       |          |          |         |         |
| System Monitoring Compounds |                 |       |       |          |          |         |         |
| 1)                          | SA Tetrachlo... | 3.473 | 4.123 | 38539196 | 386.2E6  | 16.017  | 16.456  |
| 27)                         | SA Decachlor... | 8.244 | 9.319 | 78368420 | 289.2E6  | 30.868  | 31.310  |
| Target Compounds            |                 |       |       |          |          |         |         |
| 2)                          | A alpha-BHC     | 3.914 | 4.528 | 155.8E6  | 1208.2E6 | 41.537  | 40.030  |
| 3)                          | MA gamma-BHC... | 4.198 | 4.822 | 147.9E6  | 1058.5E6 | 40.614  | 40.902  |
| 4)                          | MA Heptachlor   | 4.498 | 5.338 | 144.5E6  | 758.8E6  | 41.485  | 37.862  |
| 5)                          | MB Aldrin       | 4.747 | 5.651 | 149.1E6  | 656.4E6  | 41.262  | 37.718  |
| 6)                          | B beta-BHC      | 4.447 | 4.997 | 61415794 | 427.3E6  | 39.201  | 31.948m |
| 7)                          | B delta-BHC     | 4.653 | 5.223 | 152.5E6  | 898.2E6  | 43.776  | 39.599  |
| 8)                          | B Heptachlo...  | 5.192 | 6.046 | 136.5E6  | 557.3E6  | 40.995  | 37.531  |
| 9)                          | A Endosulfan I  | 5.531 | 6.411 | 127.0E6  | 499.8E6  | 42.143  | 37.687  |
| 10)                         | B trans-Chl...  | 5.418 | 6.283 | 141.9E6  | 561.6E6  | 40.765  | 37.300  |
| 11)                         | B cis-Chlor...  | 5.478 | 6.356 | 138.4E6  | 527.6E6  | 40.493  | 36.528  |
| 12)                         | B 4,4'-DDE      | 5.644 | 6.511 | 269.7E6  | 1043.0E6 | 83.836  | 76.045  |
| 13)                         | MA Dieldrin     | 5.776 | 6.672 | 293.6E6  | 1091.5E6 | 87.666  | 78.827  |
| 14)                         | MA Endrin       | 6.035 | 6.895 | 254.0E6  | 880.0E6  | 91.616  | 84.285  |
| 15)                         | B Endosulfa...  | 6.308 | 7.109 | 235.3E6  | 879.2E6  | 85.789  | 76.329  |
| 16)                         | A 4,4'-DDD      | 6.161 | 7.011 | 213.5E6  | 885.4E6  | 81.993  | 80.959  |
| 17)                         | MA 4,4'-DDT     | 6.402 | 7.312 | 237.2E6  | 938.6E6  | 88.635  | 83.867  |
| 18)                         | B Endrin al...  | 6.478 | 7.235 | 165.8E6  | 664.5E6  | 72.378  | 68.351  |
| 19)                         | B Endosulfa...  | 6.691 | 7.459 | 224.6E6  | 843.1E6  | 80.170  | 74.363  |
| 20)                         | A Methoxychlor  | 6.955 | 7.771 | 586.9E6  | 2069.1E6 | 424.406 | 395.468 |
| 21)                         | B Endrin ke...  | 7.185 | 7.941 | 265.6E6  | 954.3E6  | 85.674  | 77.279  |
| -----                       |                 |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD071422\  
 Data File : PD070902.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Jul 2022 03:07  
 Operator : AR\AJ  
 Sample : N3600-03MSD  
 Misc :  
 ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 14 07:39:45 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD071422CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jul 14 05:14:58 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

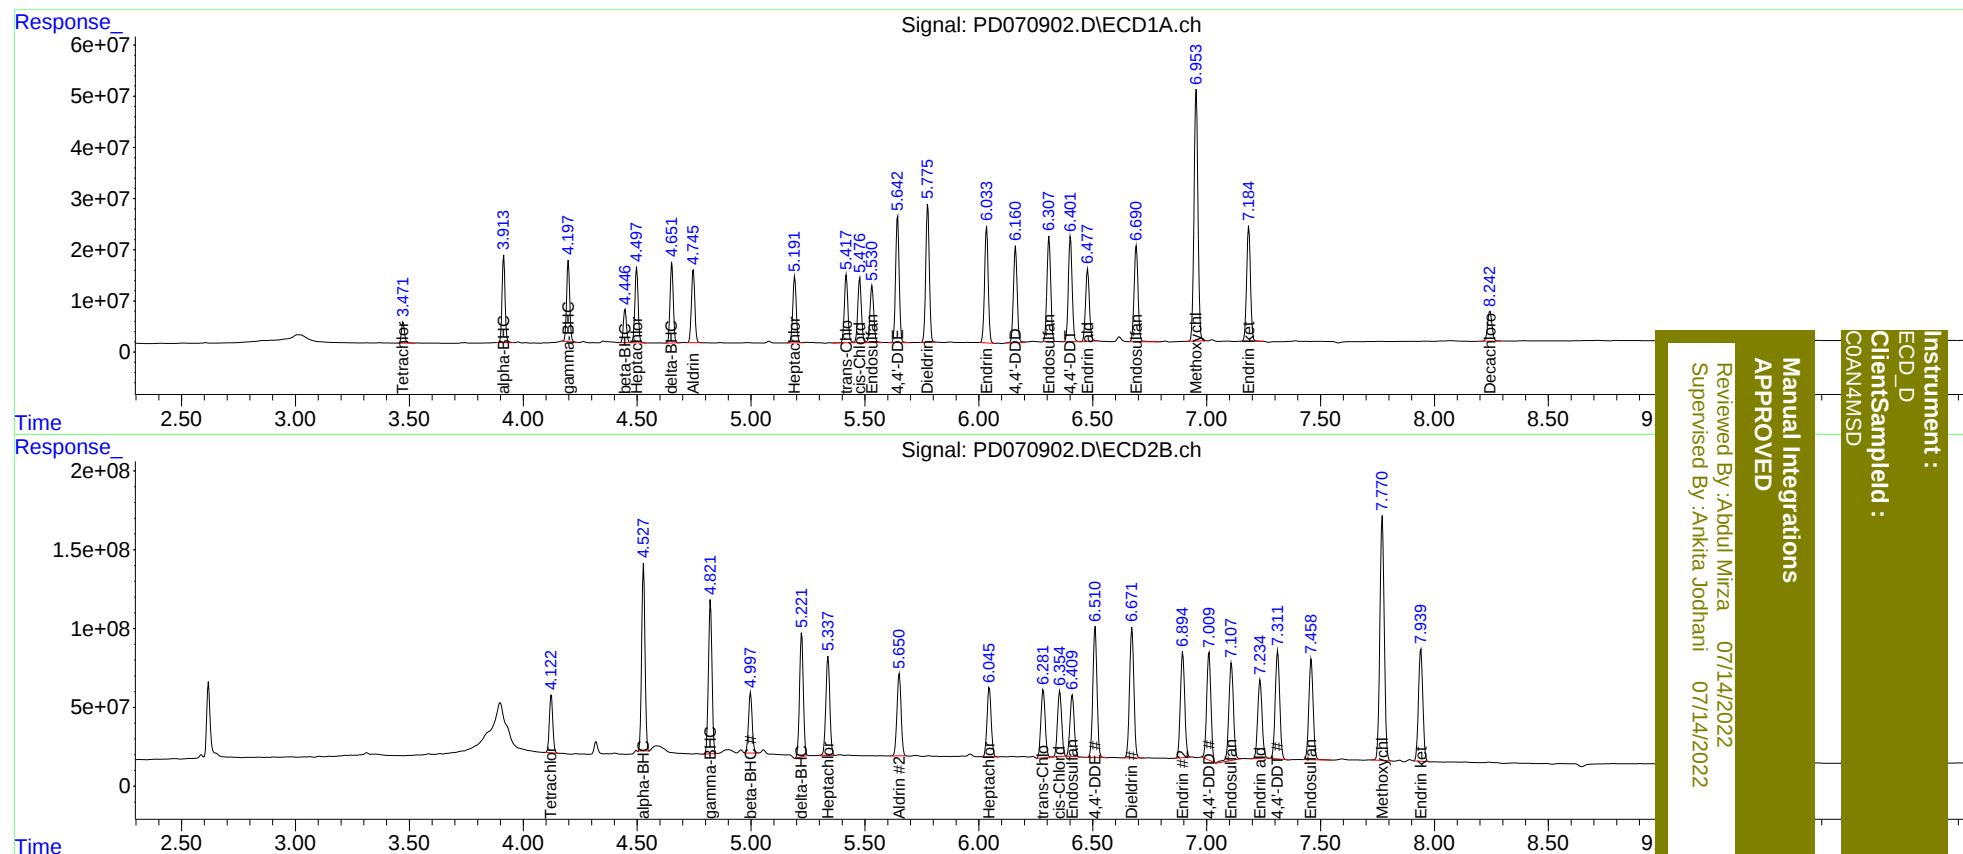

Manual Integrations  
 APPROVED  
 Reviewed By: Abdul Mirza 07/14/2022  
 Supervised By: Ankita Jodhani 07/14/2022

Instrument :  
 ECD\_D  
 Client Sampled :  
 COAN4MSD