

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
 Data File : PD070888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 23:44
 Operator : AR\AJ
 Sample : N3670-01
 Misc : PEST MDL 1 PPB
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT2-2022-03

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/14/2022
 Supervised By : Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 07:30:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.124	42144905	394.3E6	17.516	16.803
27)	SA Decachlor...	8.243	9.320	90192497	334.8E6	35.525	36.254
Target Compounds							
2)	A alpha-BHC	3.914	4.528	4718223	23185772	1.258	0.768 #
3)	MA gamma-BHC...	4.197	4.822	5063864	23699011	1.391	0.916 #
4)	MA Heptachlor	4.498	5.338	2807299	20653137	0.806	1.031 #
5)	MB Aldrin	4.746	5.650	2860672	17296989	0.792	0.994 #
6)	B beta-BHC	4.447	5.001	1101230	31576122	0.703	2.361 #
7)	B delta-BHC	4.652	5.221	2585613	20750822	0.742	0.915
8)	B Heptachlo...	5.191	6.044	2891013	16508889	0.868	1.112 #
9)	A Endosulfan I	5.531	6.410	2607962	13991726	0.865	1.055
10)	B trans-Chl...	5.417	6.282	3073339	14664918	0.883	0.974
11)	B cis-Chlor...	5.477	6.355	2999235	13939337	0.878	0.965
12)	B 4,4'-DDE	5.642	6.510	2387063	14178798	0.742	1.034 #
13)	MA Dieldrin	5.775	6.672	2751285	15365095	0.822	1.110 #
14)	MA Endrin	6.033	6.894	2344344	9251138	0.846	0.886m
15)	B Endosulfa...	6.307	7.109	2367868	11988162	0.863	1.041
16)	A 4,4'-DDD	6.160	7.009	2219174	11926078	0.852	1.090m#
17)	MA 4,4'-DDT	6.401	7.310	1952139	11760254	0.730	1.051m#
18)	B Endrin al...	6.477	7.235	2005557	9106395	0.876	0.937
19)	B Endosulfa...	6.690	7.459	2741616	10268231	0.979	0.906m
20)	A Methoxychlor	6.953	7.771	1402828	6117081	1.014	1.169
21)	B Endrin ke...	7.184	7.940	2919801	15976433	0.942	1.294m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
Data File : PD070888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 23:44
Operator : AR\AJ
Sample : N3670-01
Misc : PEST MDL 1 PPB
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 07:30:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

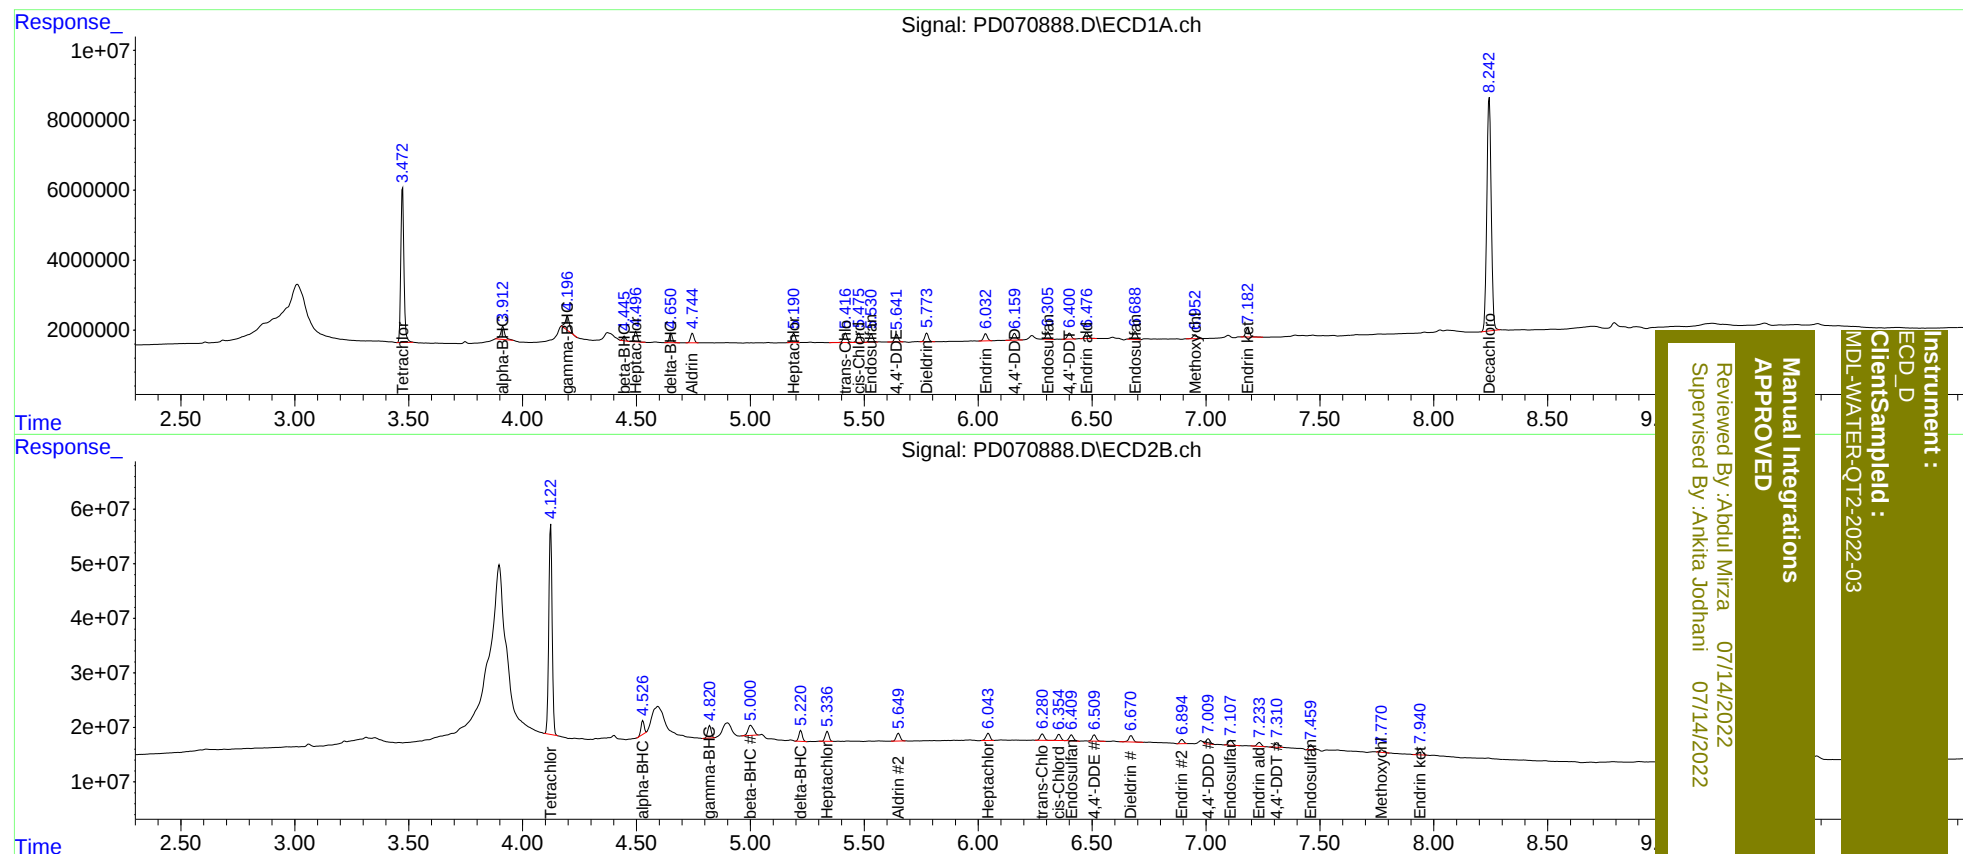

Reviewed By: Abdul Miza 07/14/2022
Supervised By: Ankita Jodhani 07/14/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT2-2022-03