

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
 Data File : PD070896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2022 01:40
 Operator : AR\AJ
 Sample : N3623-02MS
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN5MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 07:36:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.124	46954555	438.5E6	19.514	18.685
2)	SA Decachlor...	8.244	9.319	50839525	188.6E6	20.025	20.418
Target Compounds							
2)	A alpha-BHC	3.915	4.528	198.3E6	1466.8E6	52.853	48.596
3)	MA gamma-BHC...	4.199	4.822	185.5E6	1238.2E6	50.968	47.846
4)	MA Heptachlor	4.499	5.338	176.3E6	844.4E6	50.585	42.130
5)	MB Aldrin	4.747	5.651	178.1E6	741.5E6	49.279	42.606
6)	B beta-BHC	4.448	4.998	72867939	495.3E6	46.511	37.033
7)	B delta-BHC	4.653	5.222	186.4E6	1038.4E6	53.494	45.783
8)	B Heptachlo...	5.192	6.046	171.8E6	652.4E6	51.597	43.929
9)	A Endosulfan I	5.531	6.410	160.6E6	603.3E6	53.284	45.498
10)	B trans-Chl...	5.419	6.283	171.0E6	644.2E6	49.134	42.783
11)	B cis-Chlor...	5.478	6.356	168.2E6	619.3E6	49.216	42.875
12)	B 4,4'-DDE	5.644	6.511	303.7E6	1153.9E6	94.383	84.134
13)	MA Dieldrin	5.776	6.672	372.1E6	1334.8E6	111.107	96.393
14)	MA Endrin	6.034	6.895	322.2E6	1092.0E6	116.235	104.586
15)	B Endosulfa...	6.308	7.109	299.8E6	1109.5E6	109.309	96.321
16)	A 4,4'-DDD	6.161	7.011	267.8E6	1022.5E6	102.834	93.495
17)	MA 4,4'-DDT	6.403	7.312	279.7E6	1084.4E6	104.543	96.896
18)	B Endrin al...	6.478	7.235	206.9E6	812.5E6	90.306	83.573
19)	B Endosulfa...	6.691	7.459	282.4E6	1031.1E6	100.801	90.947
20)	A Methoxychlor	6.954	7.771	741.4E6	2568.3E6	536.128	490.888
21)	B Endrin ke...	7.185	7.941	337.9E6	1205.5E6	109.014	97.622

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
Data File : PD070896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2022 01:40
Operator : AR\AJ
Sample : N3623-02MS
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 07:36:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

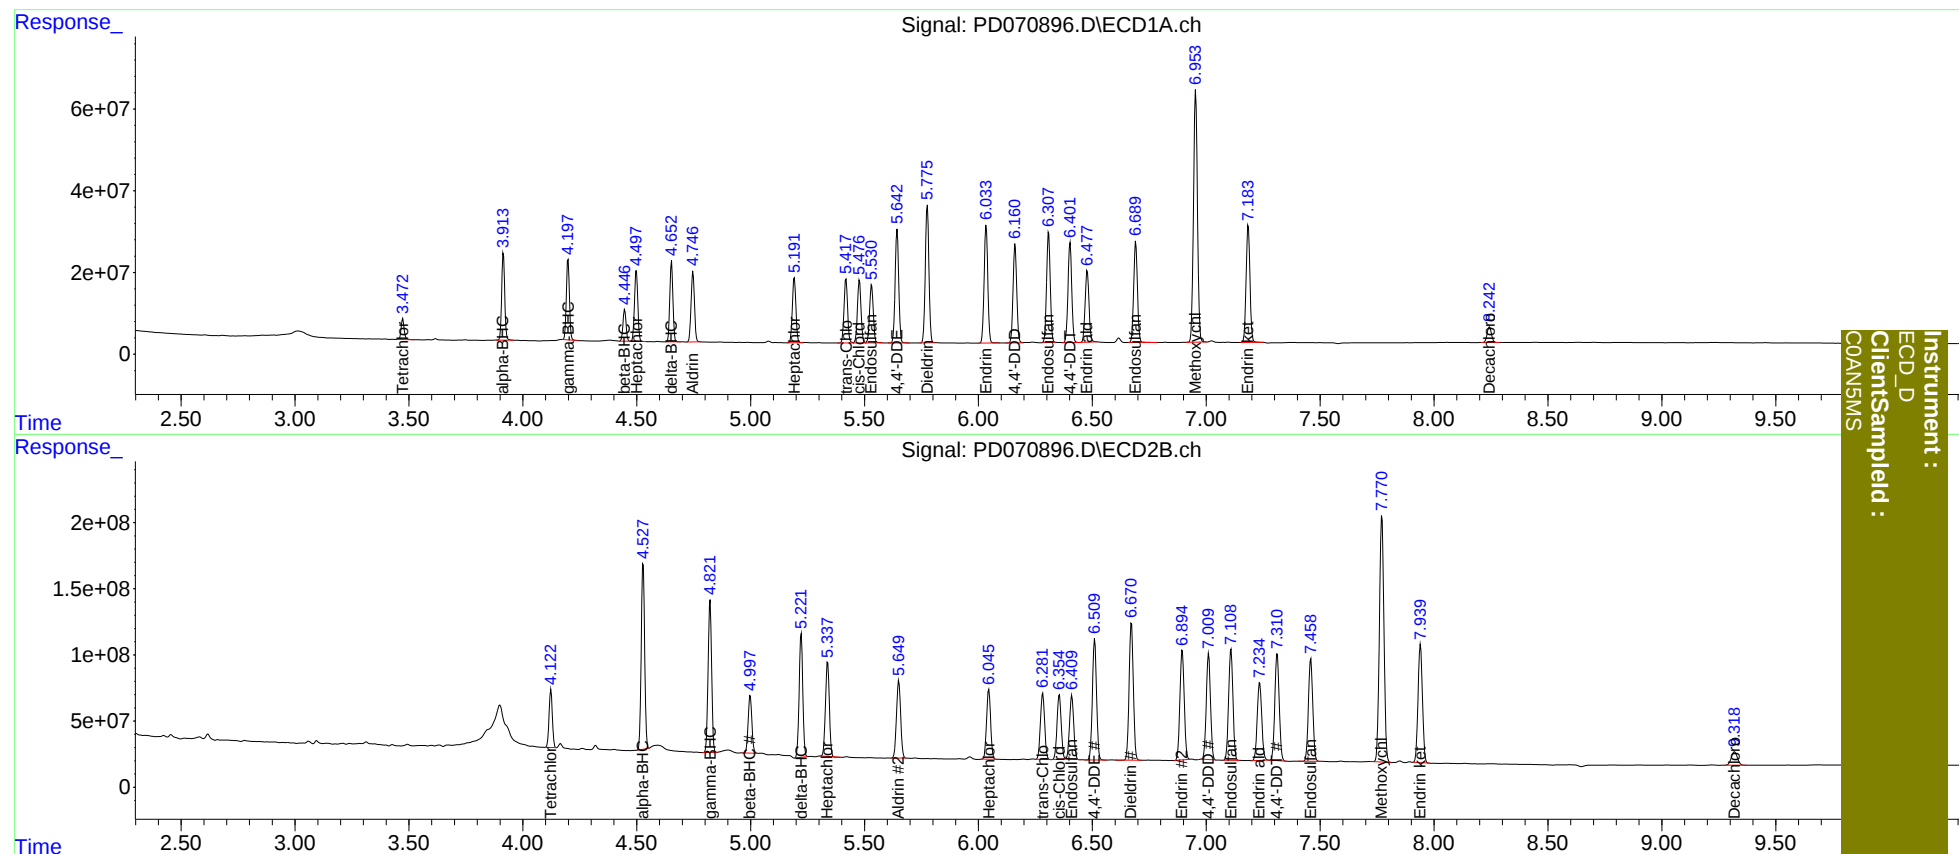

Instrument :
ECD_D
ClientSampled :
COAN5MS