

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
 Data File : PD070899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2022 02:23
 Operator : AR\AJ
 Sample : PB146173BS
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS173

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 07:38:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.124	46048490	454.2E6	19.138	19.354
2)	SA Decachlor...	8.244	9.320	101.9E6	374.2E6	40.124	40.512
Target Compounds							
2)	A alpha-BHC	3.914	4.529	17062361	147.7E6	4.548	4.895
3)	MA gamma-BHC...	4.199	4.822	16425677	139.9E6	4.512	5.406
4)	MA Heptachlor	4.499	5.338	16636667	115.6E6	4.775	5.769
5)	MB Aldrin	4.747	5.651	16965038	97613146	4.695	5.609
6)	B beta-BHC	4.448	4.999	7141189	82041662	4.558	6.135 #
7)	B delta-BHC	4.653	5.222	11731998	96761656	3.368	4.266 #
8)	B Heptachlo...	5.192	6.046	16341856	82236247	4.908	5.538
9)	A Endosulfan I	5.532	6.411	15054063	72485110	4.994	5.466
10)	B trans-Chl...	5.419	6.283	16791822	80648033	4.825	5.356
11)	B cis-Chlor...	5.478	6.356	16533068	76836410	4.838	5.320
12)	B 4,4'-DDE	5.644	6.511	30494729	150.3E6	9.478	10.960
13)	MA Dieldrin	5.776	6.672	32160137	152.9E6	9.604	11.039
14)	MA Endrin	6.034	6.896	26460798	109.8E6	9.545	10.520
15)	B Endosulfa...	6.308	7.109	27386856	128.0E6	9.986	11.110
16)	A 4,4'-DDD	6.161	7.011	25461150	119.4E6	9.776	10.913
17)	MA 4,4'-DDT	6.403	7.313	24624901	118.3E6	9.204	10.570
18)	B Endrin al...	6.478	7.236	23932765	108.6E6	10.448	11.173
19)	B Endosulfa...	6.691	7.460	24677959	105.2E6	8.810	9.282
20)	A Methoxychlor	6.954	7.772	70207390	291.1E6	50.772	55.632
21)	B Endrin ke...	7.185	7.941	32497264	137.9E6	10.483	11.170

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
Data File : PD070899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2022 02:23
Operator : AR\AJ
Sample : PB146173BS
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 07:38:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

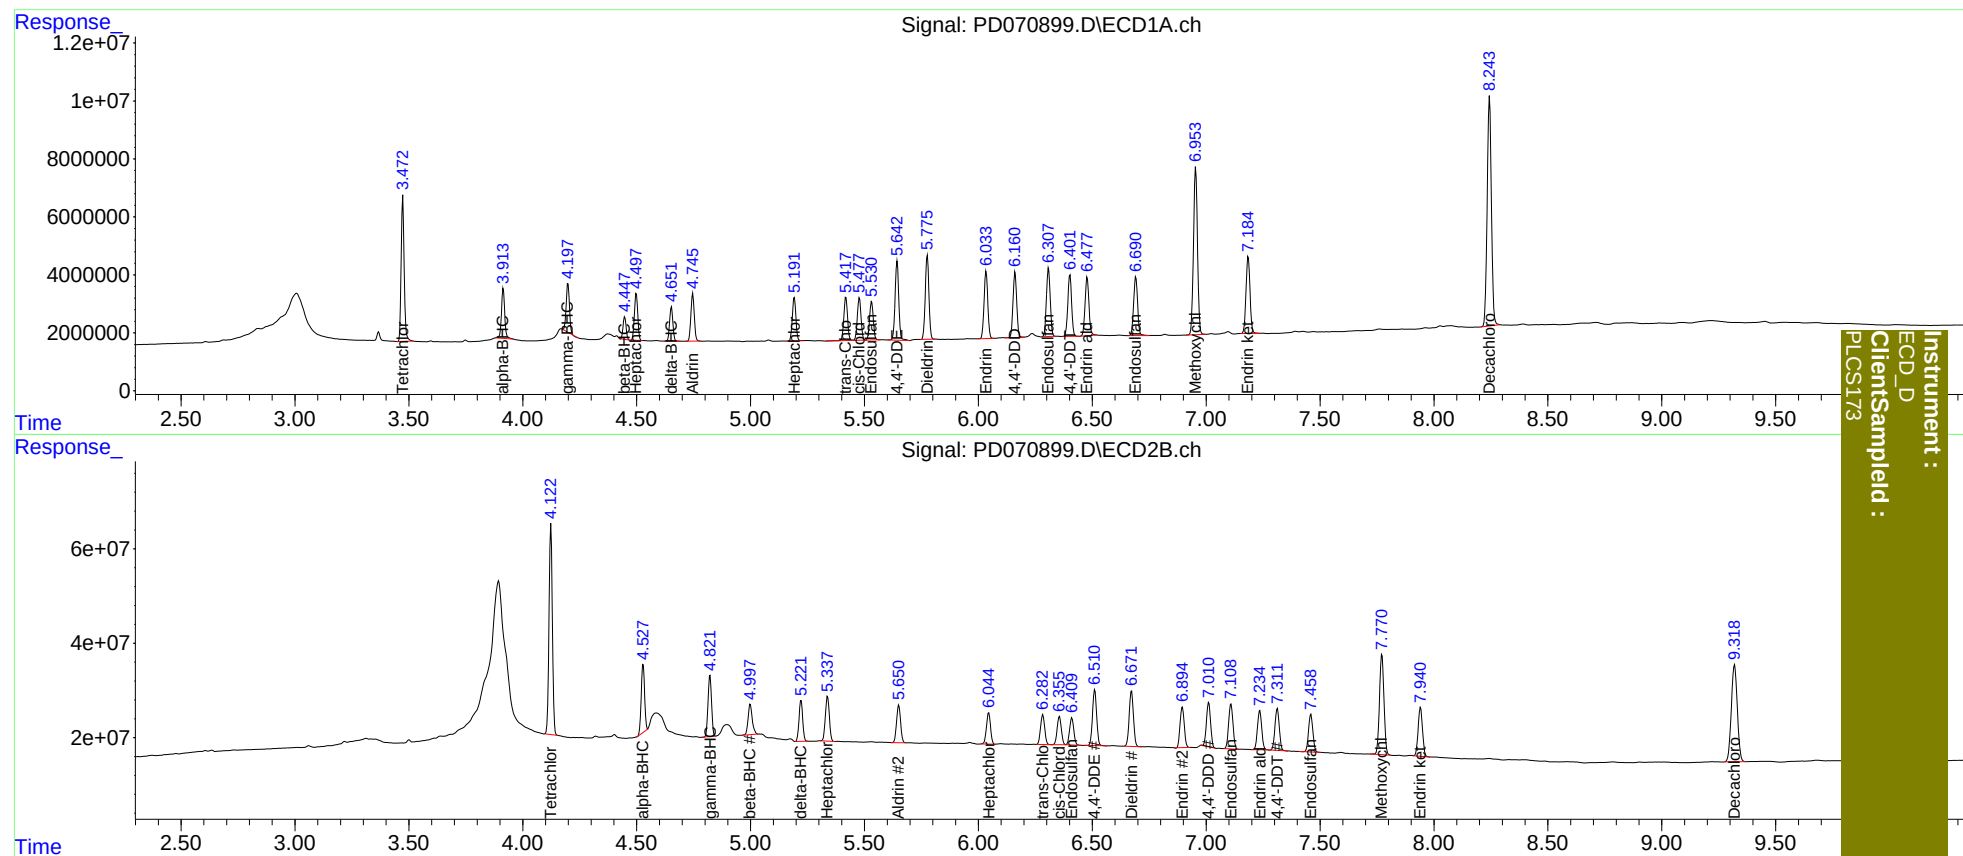

Instrument :
ECD_D
ClientSampled :
PLCS173