

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
 Data File : PD070902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2022 03:07
 Operator : AR\AJ
 Sample : N3600-03MSD
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/14/2022
 Supervised By : Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 07:39:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.123	38539196	386.2E6	16.017	16.456
27)	SA Decachlor...	8.244	9.319	78368420	289.2E6	30.868	31.310
Target Compounds							
2)	A alpha-BHC	3.914	4.528	155.8E6	1208.2E6	41.537	40.030
3)	MA gamma-BHC...	4.198	4.822	147.9E6	1058.5E6	40.614	40.902
4)	MA Heptachlor	4.498	5.338	144.5E6	758.8E6	41.485	37.862
5)	MB Aldrin	4.747	5.651	149.1E6	656.4E6	41.262	37.718
6)	B beta-BHC	4.447	4.997	61415794	427.3E6	39.201	31.948m
7)	B delta-BHC	4.653	5.223	152.5E6	898.2E6	43.776	39.599
8)	B Heptachlo...	5.192	6.046	136.5E6	557.3E6	40.995	37.531
9)	A Endosulfan I	5.531	6.411	127.0E6	499.8E6	42.143	37.687
10)	B trans-Chl...	5.418	6.283	141.9E6	561.6E6	40.765	37.300
11)	B cis-Chlor...	5.478	6.356	138.4E6	527.6E6	40.493	36.528
12)	B 4,4'-DDE	5.644	6.511	269.7E6	1043.0E6	83.836	76.045
13)	MA Dieldrin	5.776	6.672	293.6E6	1091.5E6	87.666	78.827
14)	MA Endrin	6.035	6.895	254.0E6	880.0E6	91.616	84.285
15)	B Endosulfa...	6.308	7.109	235.3E6	879.2E6	85.789	76.329
16)	A 4,4'-DDD	6.161	7.011	213.5E6	885.4E6	81.993	80.959
17)	MA 4,4'-DDT	6.402	7.312	237.2E6	938.6E6	88.635	83.867
18)	B Endrin al...	6.478	7.235	165.8E6	664.5E6	72.378	68.351
19)	B Endosulfa...	6.691	7.459	224.6E6	843.1E6	80.170	74.363
20)	A Methoxychlor	6.955	7.771	586.9E6	2069.1E6	424.406	395.468
21)	B Endrin ke...	7.185	7.941	265.6E6	954.3E6	85.674	77.279

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071422\
Data File : PD070902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2022 03:07
Operator : AR\AJ
Sample : N3600-03MSD
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 07:39:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

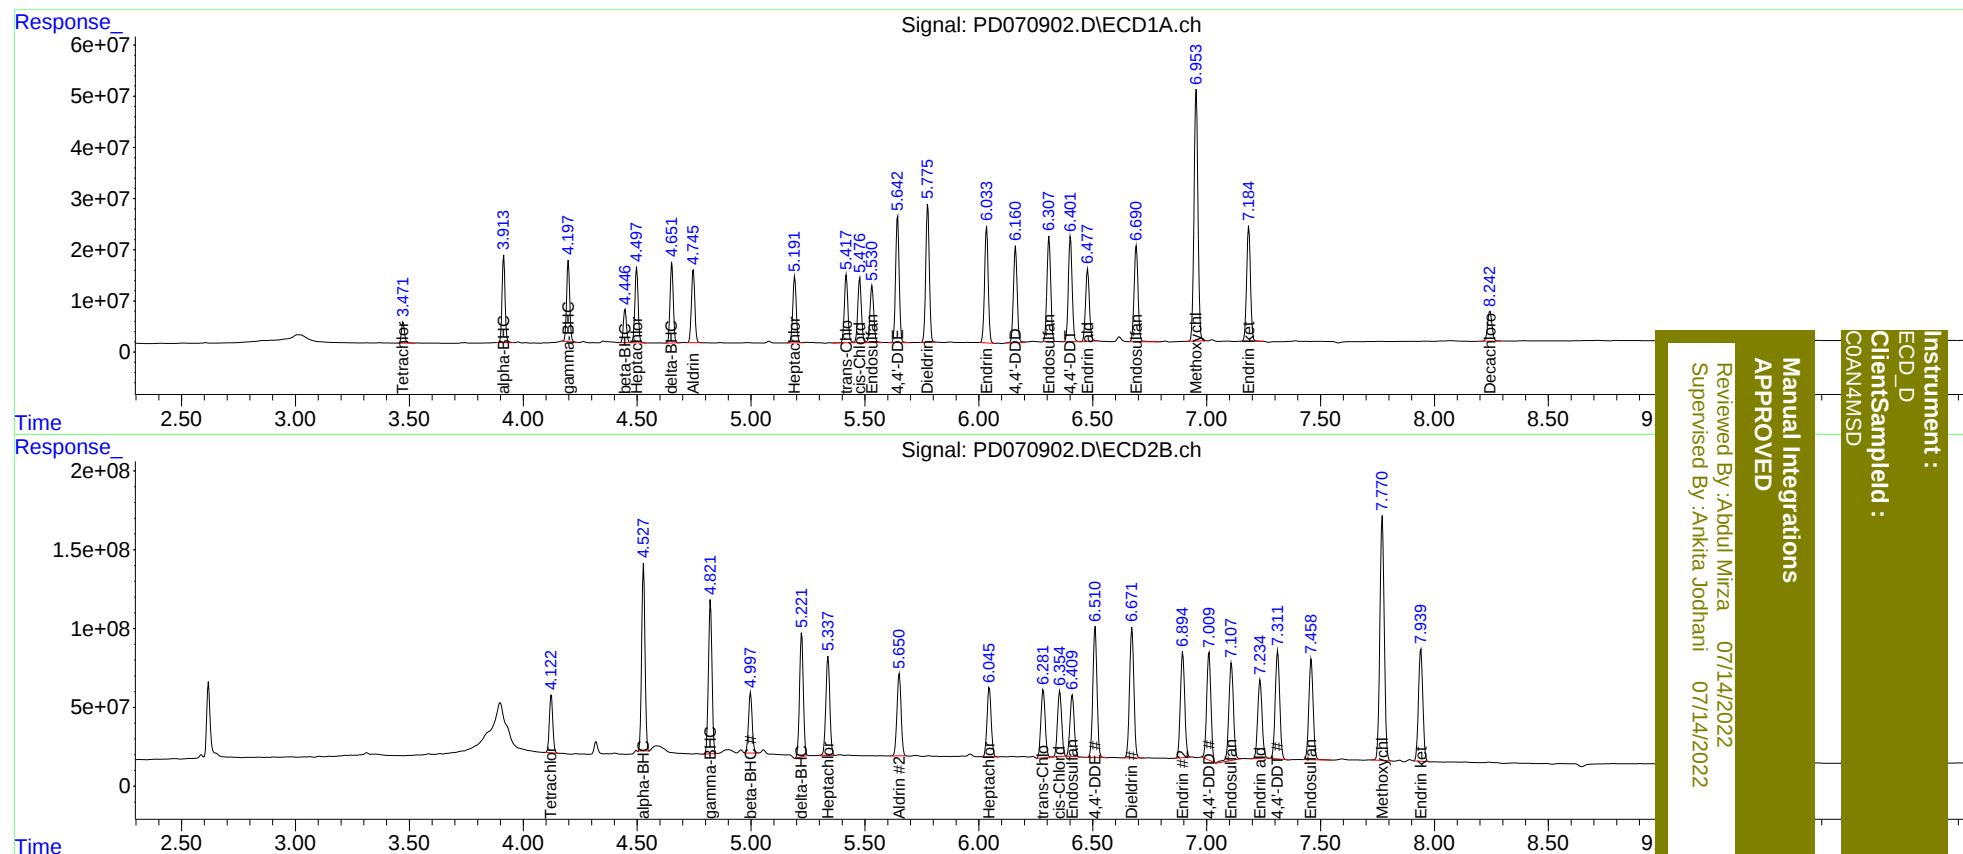

Reviewed By: Abdul Mirza 07/14/2022
Supervised By: Ankita Jodhani 07/14/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COAN4MSD