

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 22:28
 Operator : AR\AJ
 Sample : 03418-23MSD
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 01:32:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.764	101.4E6	12765388	47.668	11.959 #
27)	SA Decachlor...	9.082	7.904	57705310	25357601	23.752	23.655
Target Compounds							
2)	A alpha-BHC	4.000	3.265	186.3E6	84577655	52.575	53.450
3)	MA gamma-BHC...	4.336	3.595	268.8E6	69273593	81.044	46.240 #
4)	MA Heptachlor	4.925	3.934	162.7E6	149.0E6	46.802	99.665 #
5)	MB Aldrin	5.267	4.214	187.1E6	112.5E6	54.713	74.743 #
6)	B beta-BHC	4.510f	3.892	104.2E6	28641918	68.524	39.981 #
7)	B delta-BHC	4.780	4.122	207.1E6	93312573	61.748	61.136
8)	B Heptachlo...	5.694	4.716	176.1E6	75163258	58.776	53.426
9)	A Endosulfan I	6.082	5.086	154.0E6	58266720	54.061	47.028
10)	B trans-Chl...	5.951	4.966	148.2E6	71416534	48.188	52.814
11)	B cis-Chlor...	6.031	5.031	161.8E6	71804512	51.038	50.895
12)	B 4,4'-DDE	6.203	5.219	302.4E6	137.4E6	103.814	113.700
13)	MA Dieldrin	6.357	5.351	339.9E6	156.3E6	107.719	112.103
14)	MA Endrin	6.588	5.627	288.4E6	130.6E6	111.871	105.634
15)	B Endosulfa...	6.807	5.921	269.7E6	128.9E6	101.420	107.173
16)	A 4,4'-DDD	6.721	5.774	255.7E6	106.8E6	113.145	112.646
17)	MA 4,4'-DDT	7.036	6.024	247.4E6	118.9E6	110.816	126.892
18)	B Endrin al...	6.937	6.100	188.3E6	80445373	100.713	95.904
19)	B Endosulfa...	7.172	6.323	265.8E6	115.5E6	106.437	103.521
20)	A Methoxychlor	7.512	6.600	700.3E6	291.2E6	529.002	545.602
21)	B Endrin ke...	7.659	6.829	312.8E6	124.5E6	112.968	97.263
22)	Toxaphene-1	6.247	4.966	664534	71416534	29.912	9706.772 #
23)	Toxaphene-2	6.464	5.695	2839938	693626	102.989	87.405
24)	Toxaphene-3	6.668	5.921f	-2393198	128.9E6	N.D.	14057.541
25)	Toxaphene-4	7.172	6.600	265.8E6	291.2E6	4432.404	11605.076 #
26)	Toxaphene-5	0.000	6.707	0	601228	N.D.	16.237

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 22:28
Operator : AR\AJ
Sample : 03418-23MSD
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 01:32:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

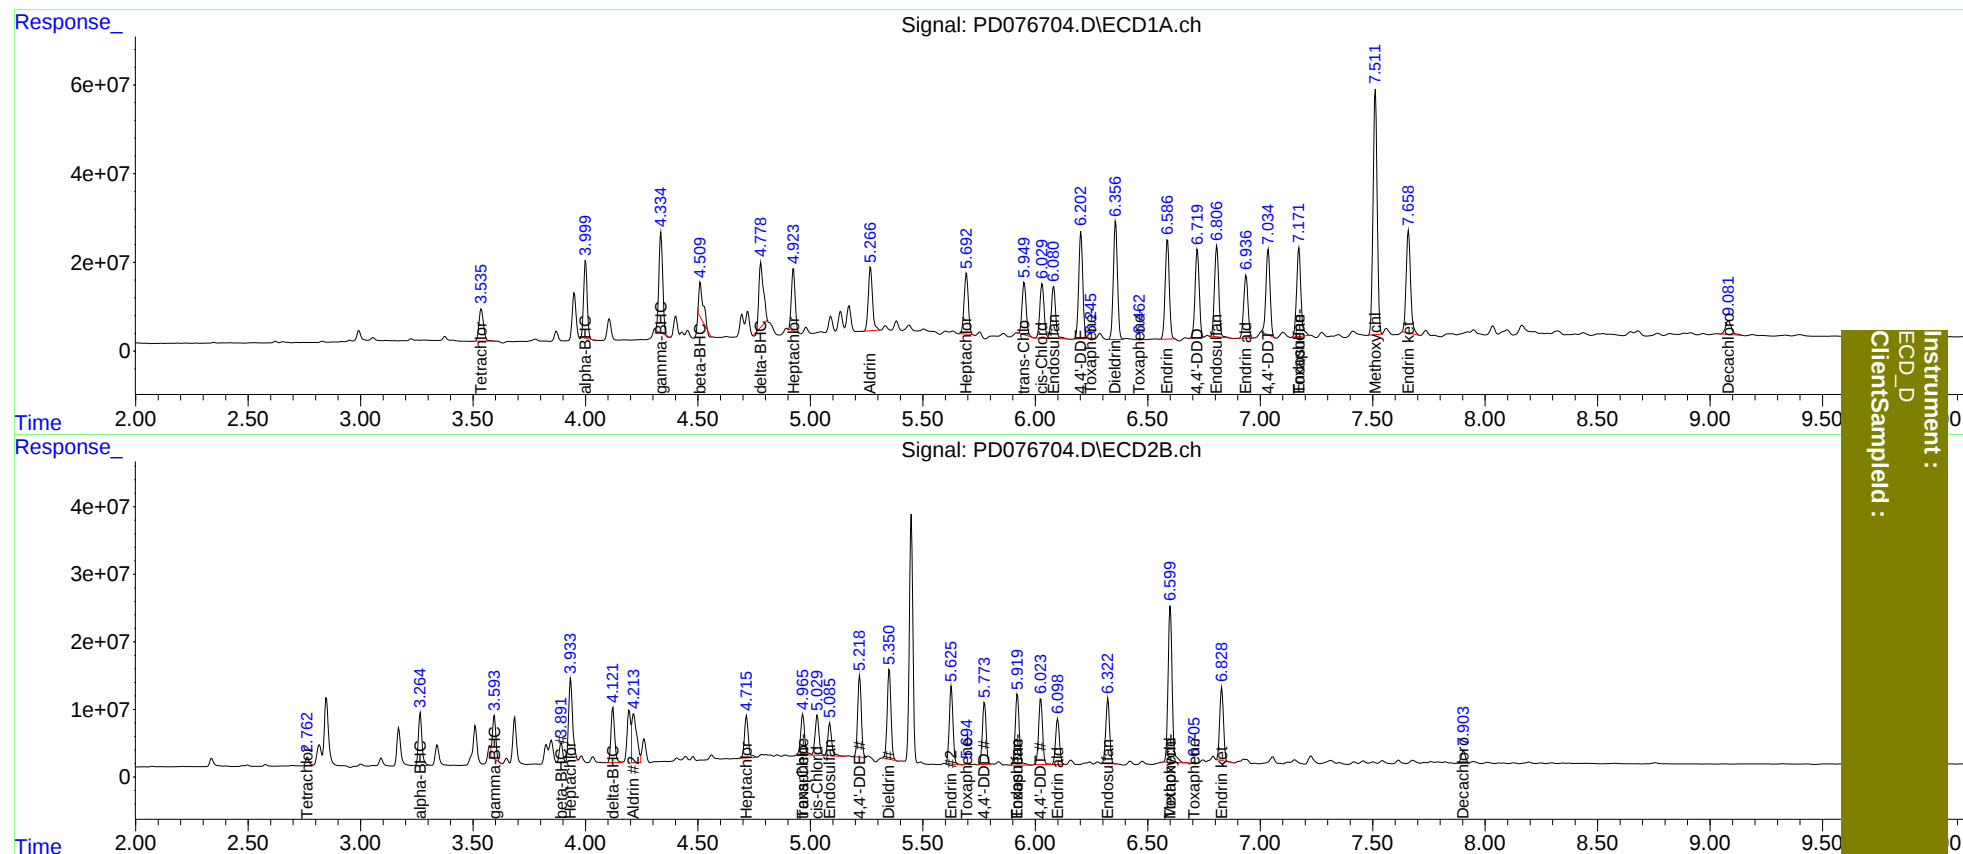

Instrument :
ECD_D
ClientSampled :