

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 04:58
 Operator : AR\AJ
 Sample : 03444-08MS
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46Q1MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 06:52:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.764	299.7E6	14064970	140.870m	13.177 #
2)	SA Decachlor...	9.083	7.905	70966286	29343558	29.210	27.373
Target Compounds							
2)	A alpha-BHC	3.999	3.265	197.8E6	79233006	55.806m	50.073
3)	MA gamma-BHC...	4.335	3.592	345.0E6	73757734	103.997m	49.233m#
4)	MA Heptachlor	4.923	3.933	174.9E6	171.5E6	50.322m	114.693 #
5)	MB Aldrin	5.268	4.215	174.1E6	80737667	50.906	53.647m
6)	B beta-BHC	4.526	3.891	54976825	27122113	36.170m	37.860
7)	B delta-BHC	4.779	4.122	213.8E6	89095491	63.752m	58.373
8)	B Heptachlo...	5.693	4.715	180.6E6	76599942	60.275	54.447
9)	A Endosulfan I	6.081	5.086	144.5E6	51757397	50.744	41.774
10)	B trans-Chl...	5.950	4.965	161.4E6	79927873	52.496m	59.108m
11)	B cis-Chlor...	6.031	5.030	159.9E6	64900646	50.451	46.002
12)	B 4,4'-DDE	6.203	5.219	307.9E6	127.8E6	105.680	105.709
13)	MA Dieldrin	6.357	5.351	341.0E6	170.7E6	108.069	122.399
14)	MA Endrin	6.588	5.627	282.4E6	125.5E6	109.544	101.460
15)	B Endosulfa...	6.808	5.921	265.4E6	118.6E6	99.819	98.638
16)	A 4,4'-DDD	6.722	5.774	259.9E6	103.5E6	115.018	109.204
17)	MA 4,4'-DDT	7.035	6.025	259.4E6	113.4E6	116.160m	121.084
18)	B Endrin al...	6.938	6.099	179.3E6	79534698	95.901	94.819m
19)	B Endosulfa...	7.173	6.324	250.1E6	111.9E6	100.159	100.299
20)	A Methoxychlor	7.513	6.600	674.2E6	283.5E6	509.356	531.321m
21)	B Endrin ke...	7.658	6.830	268.3E6	128.6E6	96.901m	100.486

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 04:58
Operator : AR\AJ
Sample : 03444-08MS
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 06:52:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

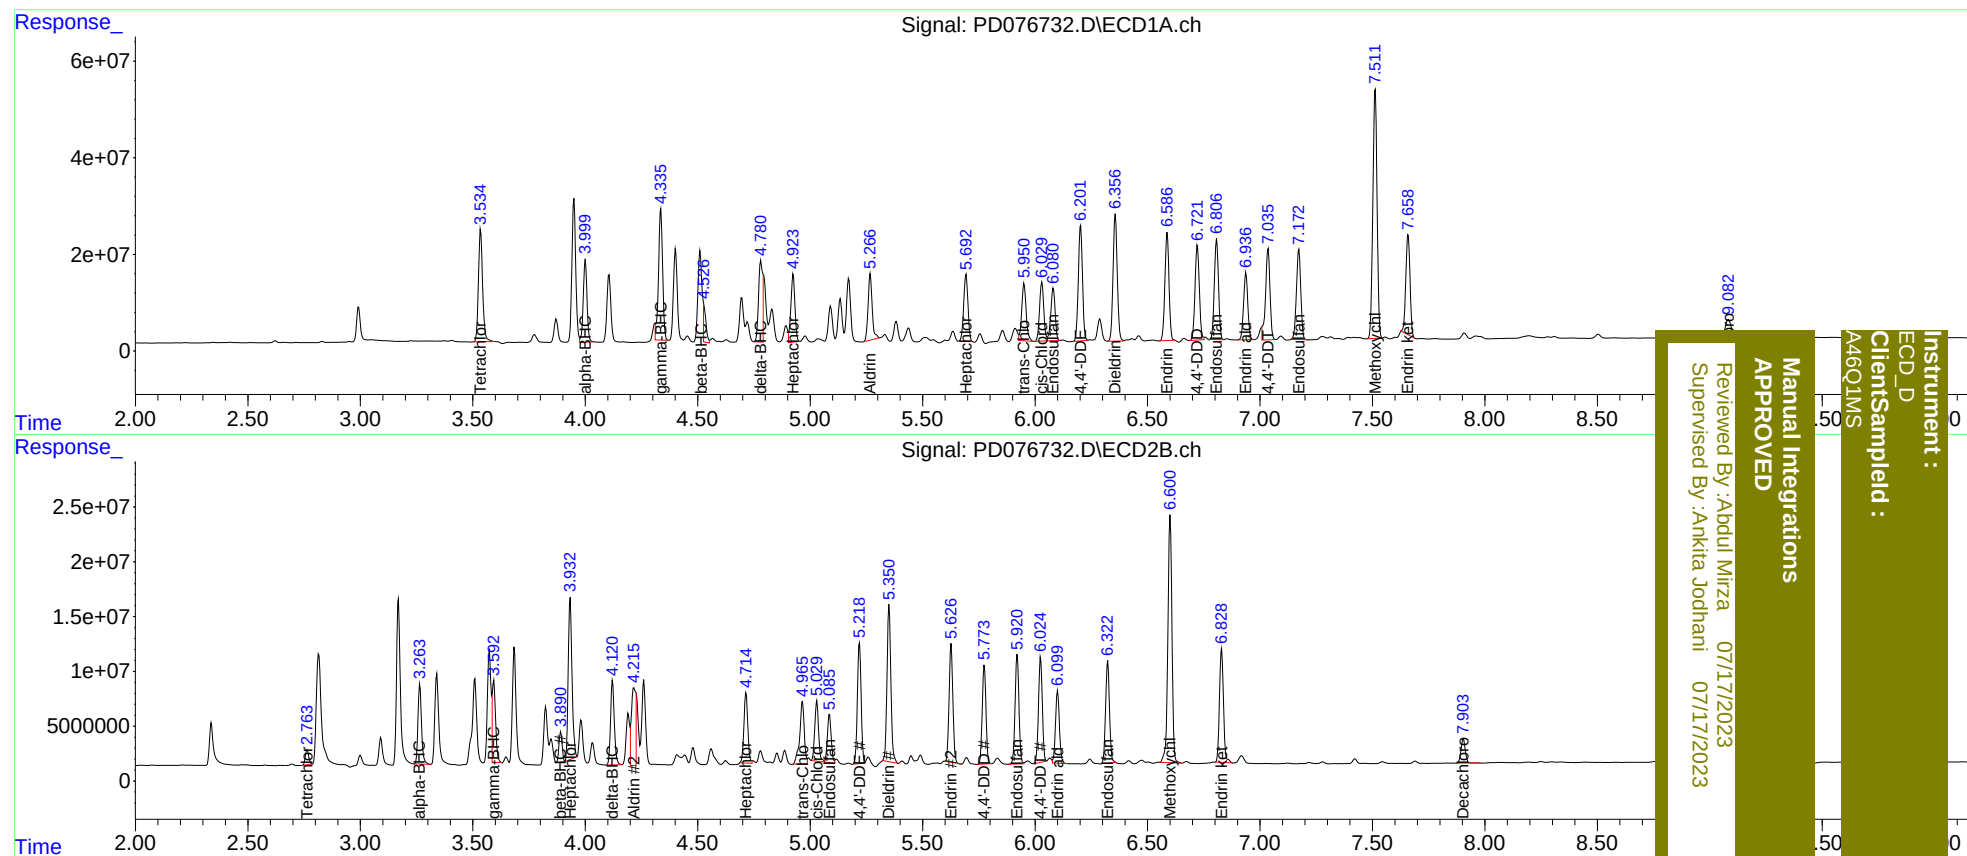

280.604

Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
A46Q1MS