

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 20:28
 Operator : AR\AJ
 Sample : 03418-14
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46J3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 01:30:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.764	61328369	17892880	28.828	16.763 #
2)	SA Decachlor...	9.082	7.904	74426869	31537657	30.635	29.420
Target Compounds							
3)	MA gamma-BHC...	4.337	3.573	80439226	24083469	24.250m	16.076m#
7)	B delta-BHC	4.795	4.130	71533008	7267372	21.331m	4.761 #
16)	A 4,4'-DDD	6.721	5.773	12653917	2757654	5.600m	2.910m#
17)	MA 4,4'-DDT	7.006	6.020	8737816	4575065	3.913m	4.884

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 20:28
Operator : AR\AJ
Sample : 03418-14
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 01:30:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

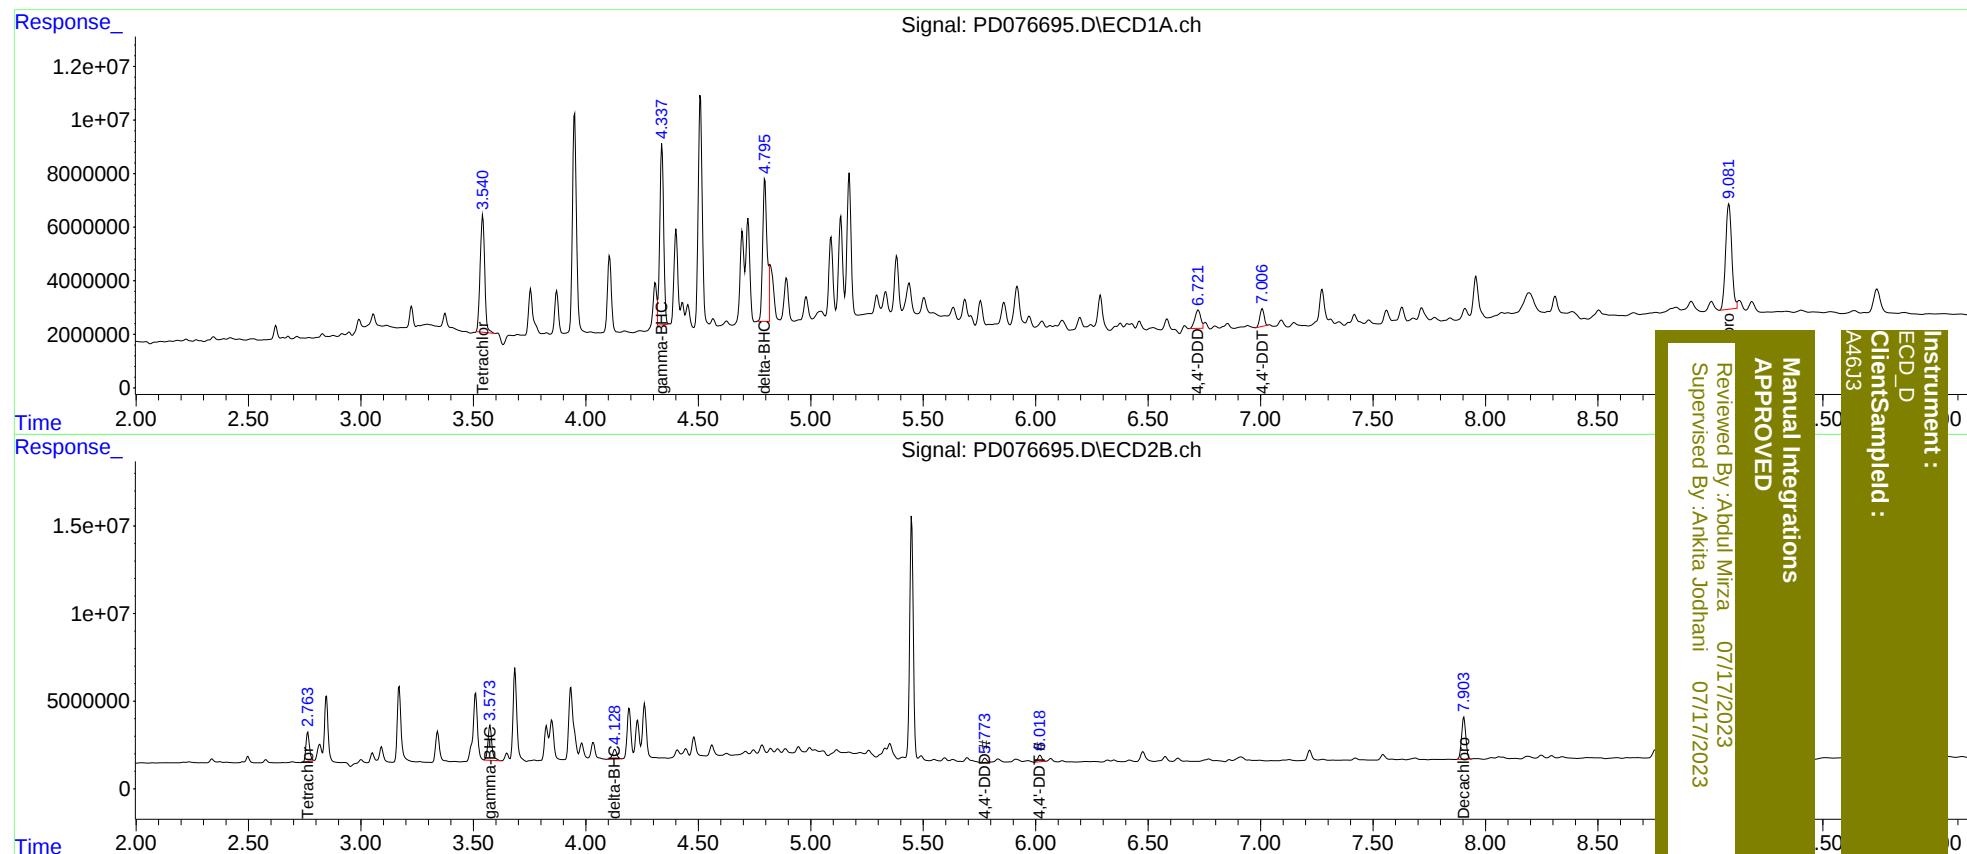

Instrument :
ECD_D
ClientSampled :
A46J3

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023