

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 20:41
 Operator : AR\AJ
 Sample : 03418-15
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46J4

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 01:30:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.764	32957008	16171600	15.492	15.150
2) SA Decachlor...	9.084	7.904	74865727	30789665	30.815	28.722
Target Compounds						
12) B 4,4'-DDE	6.198	5.219	1356914	637089	0.466	0.527m
16) A 4,4'-DDD	6.724	5.773	3690809	769881	1.633	0.812m#
17) MA 4,4'-DDT	7.008	6.021	2086900	1723363	0.935m	1.840 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 20:41
Operator : AR\AJ
Sample : 03418-15
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 01:30:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

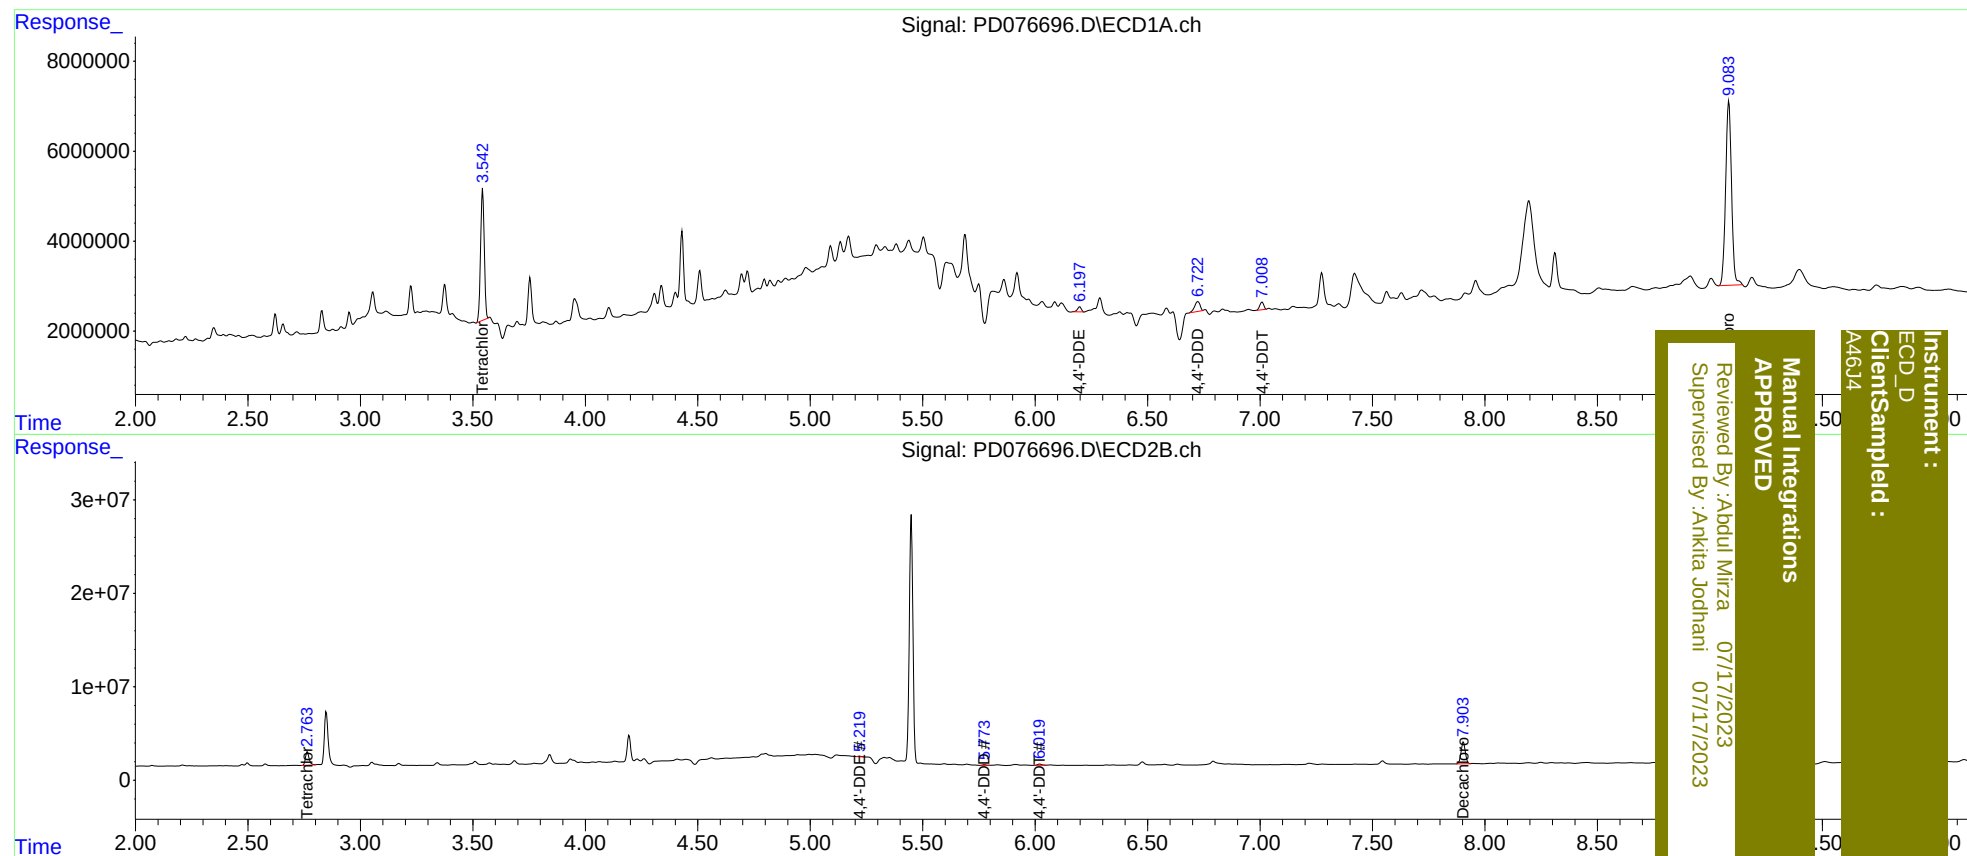

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Instrument :
ECD_D
Client Sampled :
A46J4