

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 22:15
 Operator : AR\AJ
 Sample : 03418-22MS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46K6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 01:31:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.764	98375089	12780568	46.243m	11.973 #
27)	SA Decachlor...	9.084	7.905	57058186	25071057	23.486	23.388
Target Compounds							
2)	A alpha-BHC	3.999	3.266	202.9E6	84311537	57.237m	53.282
3)	MA gamma-BHC...	4.334	3.593	296.7E6	82473559	89.460m	55.051m#
4)	MA Heptachlor	4.925	3.934	163.0E6	149.2E6	46.898	99.786 #
5)	MB Aldrin	5.267	4.215	188.3E6	112.0E6	55.076	74.419 #
6)	B beta-BHC	4.525	3.892	65054518	29078121	42.800m	40.590
7)	B delta-BHC	4.778	4.122	231.3E6	92519173	68.977m	60.616
8)	B Heptachlo...	5.695	4.716	172.1E6	75264623	57.432	53.498
9)	A Endosulfan I	6.082	5.087	154.6E6	60706460	54.276	48.997
10)	B trans-Chl...	5.952	4.967	150.0E6	72823925	48.768	53.855
11)	B cis-Chlor...	6.031	5.031	163.4E6	72553920	51.548	51.427
12)	B 4,4'-DDE	6.203	5.220	307.0E6	137.1E6	105.376	113.443
13)	MA Dieldrin	6.357	5.351	342.6E6	156.7E6	108.589	112.369
14)	MA Endrin	6.588	5.627	289.7E6	130.2E6	112.389	105.311
15)	B Endosulfa...	6.808	5.921	269.8E6	128.8E6	101.479	107.093
16)	A 4,4'-DDD	6.722	5.775	258.1E6	106.8E6	114.218	112.646
17)	MA 4,4'-DDT	7.035	6.025	287.8E6	118.0E6	128.894m	125.984
18)	B Endrin al...	6.938	6.101	190.5E6	80827601	101.886	96.360
19)	B Endosulfa...	7.173	6.323	267.5E6	115.2E6	107.125	103.210
20)	A Methoxychlor	7.513	6.601	710.6E6	291.2E6	536.827	545.581
21)	B Endrin ke...	7.658	6.830	337.5E6	123.4E6	121.898m	96.408

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 22:15
Operator : AR\AJ
Sample : 03418-22MS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 01:31:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

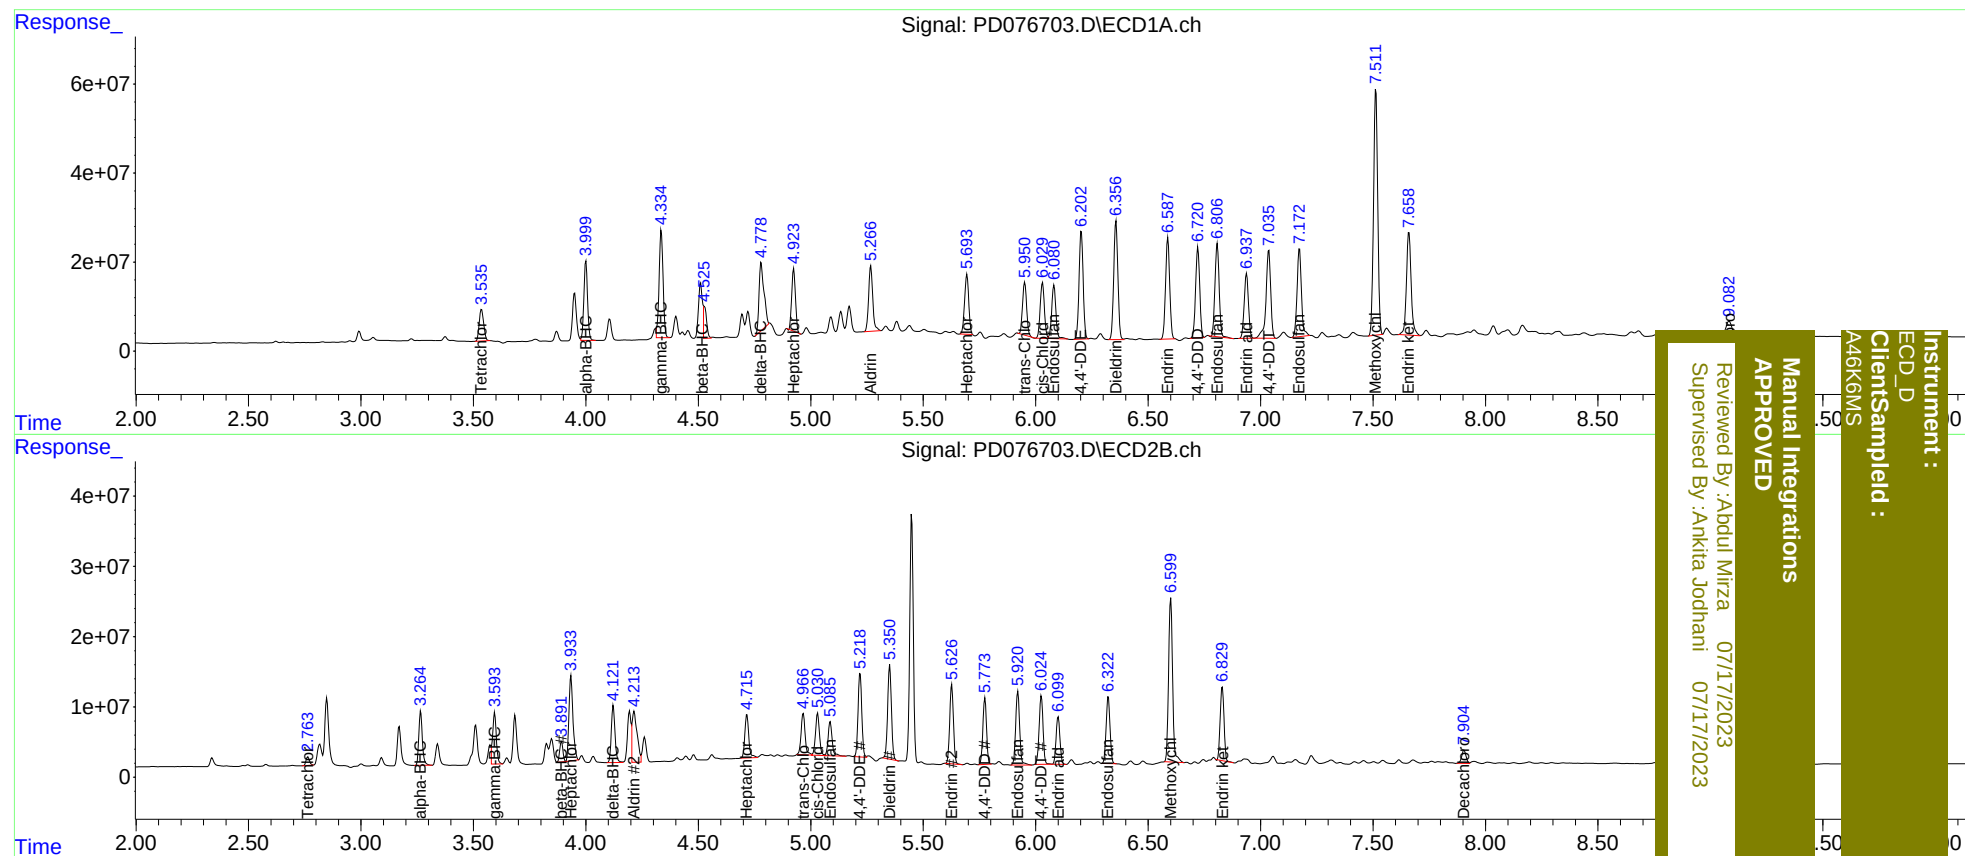

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Instrument :
ECD_D
Client Sampled :
A46K6MS