

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 00:56
 Operator : AR\AJ
 Sample : 03437-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46K7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 06:46:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.764	73215997	16973774	34.416m	15.902 #
2)	SA Decachlor...	9.083	7.904	68689181	29976727	28.273	27.964
Target Compounds							
3)	MA gamma-BHC...	4.337	3.572	10559143	10303469	3.183m	6.878m#
7)	B delta-BHC	4.794	4.129	5158719	1908531	1.538m	1.250m
10)	B trans-Chl...	5.971	4.945	1470803	1168753	0.478m	0.864m#
17)	MA 4,4'-DDT	7.007	6.019	1907651	1617300	0.854m	1.726 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 00:56
Operator : AR\AJ
Sample : 03437-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 06:46:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

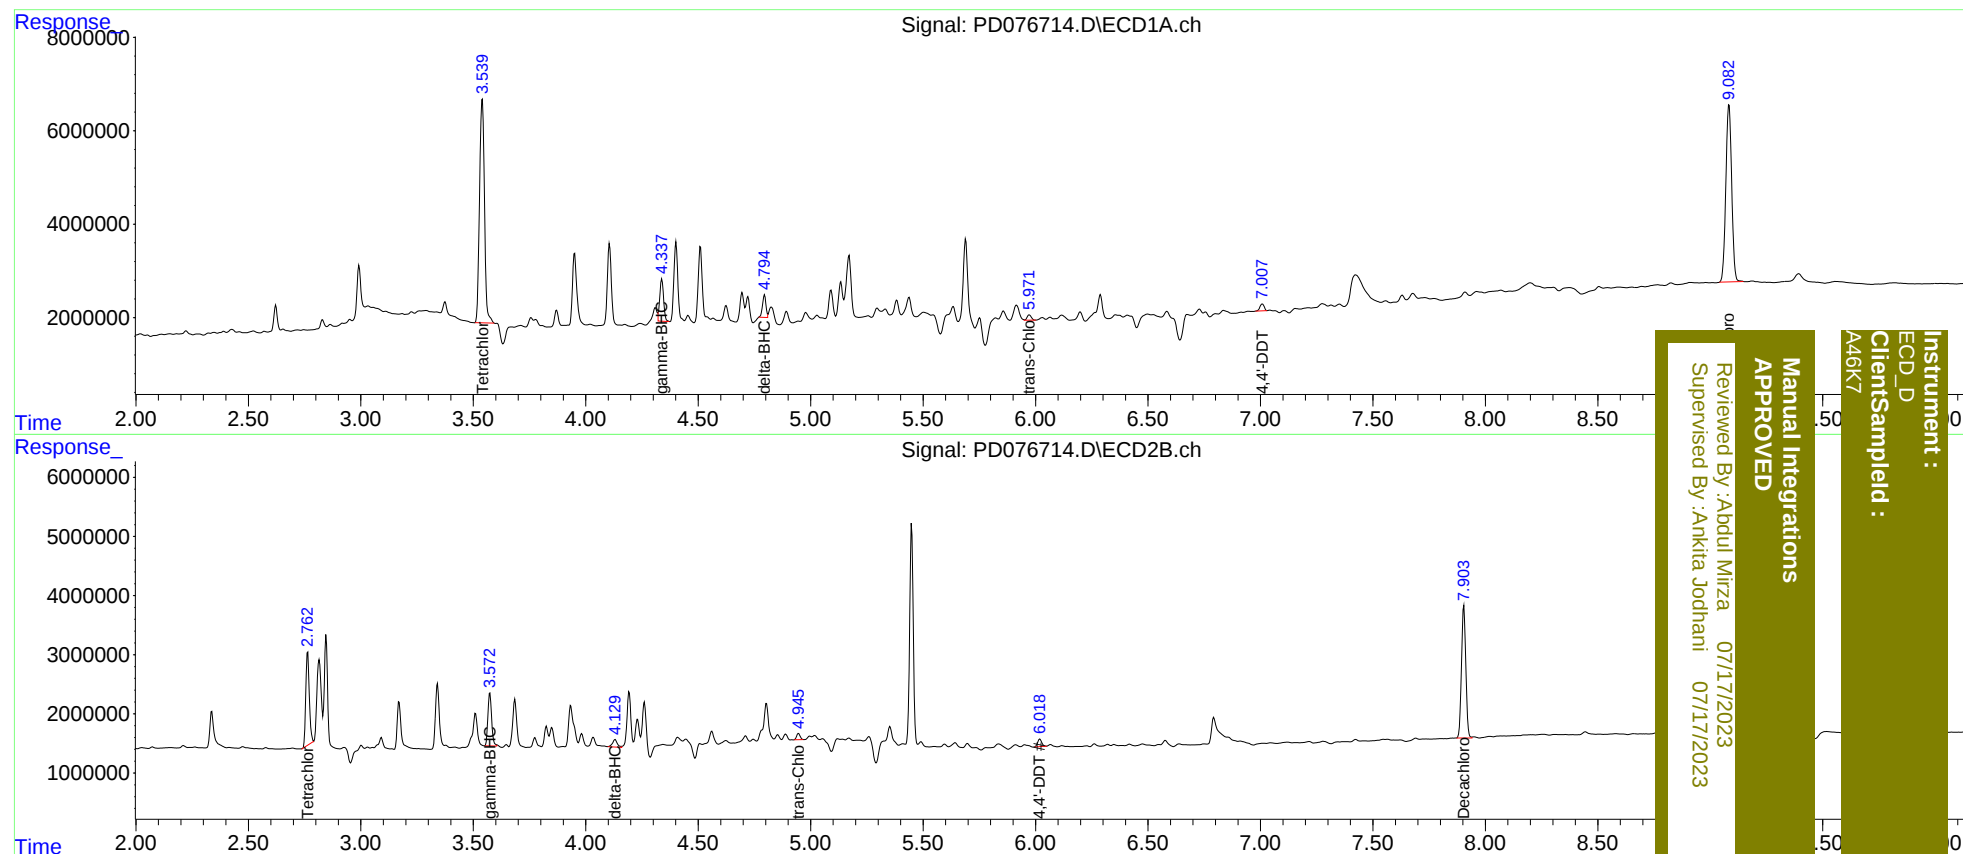

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Instrument :
ECD_D
ClientSampled :
A46K7