

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 01:23
 Operator : AR\AJ
 Sample : 03437-12MSD
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46K7MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 06:47:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.764	69227487	15730465	32.542m	14.737 #
2)	SA Decachlor...	9.082	7.904	66488178	28086639	27.367	26.201
Target Compounds							
2)	A alpha-BHC	4.000	3.265	219.7E6	93808091	61.972	59.284
3)	MA gamma-BHC...	4.332	3.593	208.6E6	94498433	62.887m	63.078m
4)	MA Heptachlor	4.924	3.934	197.8E6	91772133	56.910	61.378
5)	MB Aldrin	5.267	4.214	201.5E6	109.8E6	58.918	72.931
6)	B beta-BHC	4.528	3.892	90046497	35598621	59.243m	49.692
7)	B delta-BHC	4.778	4.121	199.6E6	91902050	59.506	60.212
8)	B Heptachlo...	5.694	4.716	195.5E6	76949191	65.251	54.695
9)	A Endosulfan I	6.081	5.086	169.4E6	58616347	59.474	47.310
10)	B trans-Chl...	5.951	4.966	172.0E6	75005834	55.939	55.468
11)	B cis-Chlor...	6.030	5.031	180.1E6	75575349	56.806	53.568
12)	B 4,4'-DDE	6.202	5.219	345.5E6	149.9E6	118.586	124.058
13)	MA Dieldrin	6.357	5.351	380.4E6	163.7E6	120.566	117.409
14)	MA Endrin	6.588	5.627	316.2E6	144.9E6	122.663	117.164
15)	B Endosulfa...	6.807	5.921	310.2E6	136.8E6	116.658	113.733
16)	A 4,4'-DDD	6.721	5.774	287.6E6	120.0E6	127.262	126.635
17)	MA 4,4'-DDT	7.036	6.025	283.9E6	122.3E6	127.144	130.599
18)	B Endrin al...	6.937	6.100	209.1E6	91504577	111.809	109.089
19)	B Endosulfa...	7.172	6.324	287.6E6	126.2E6	115.153	113.091
20)	A Methoxychlor	7.511	6.601	758.7E6	311.1E6	573.152	582.923
21)	B Endrin ke...	7.659	6.830	319.4E6	145.0E6	115.343	113.306

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 01:23
Operator : AR\AJ
Sample : 03437-12MSD
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 06:47:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

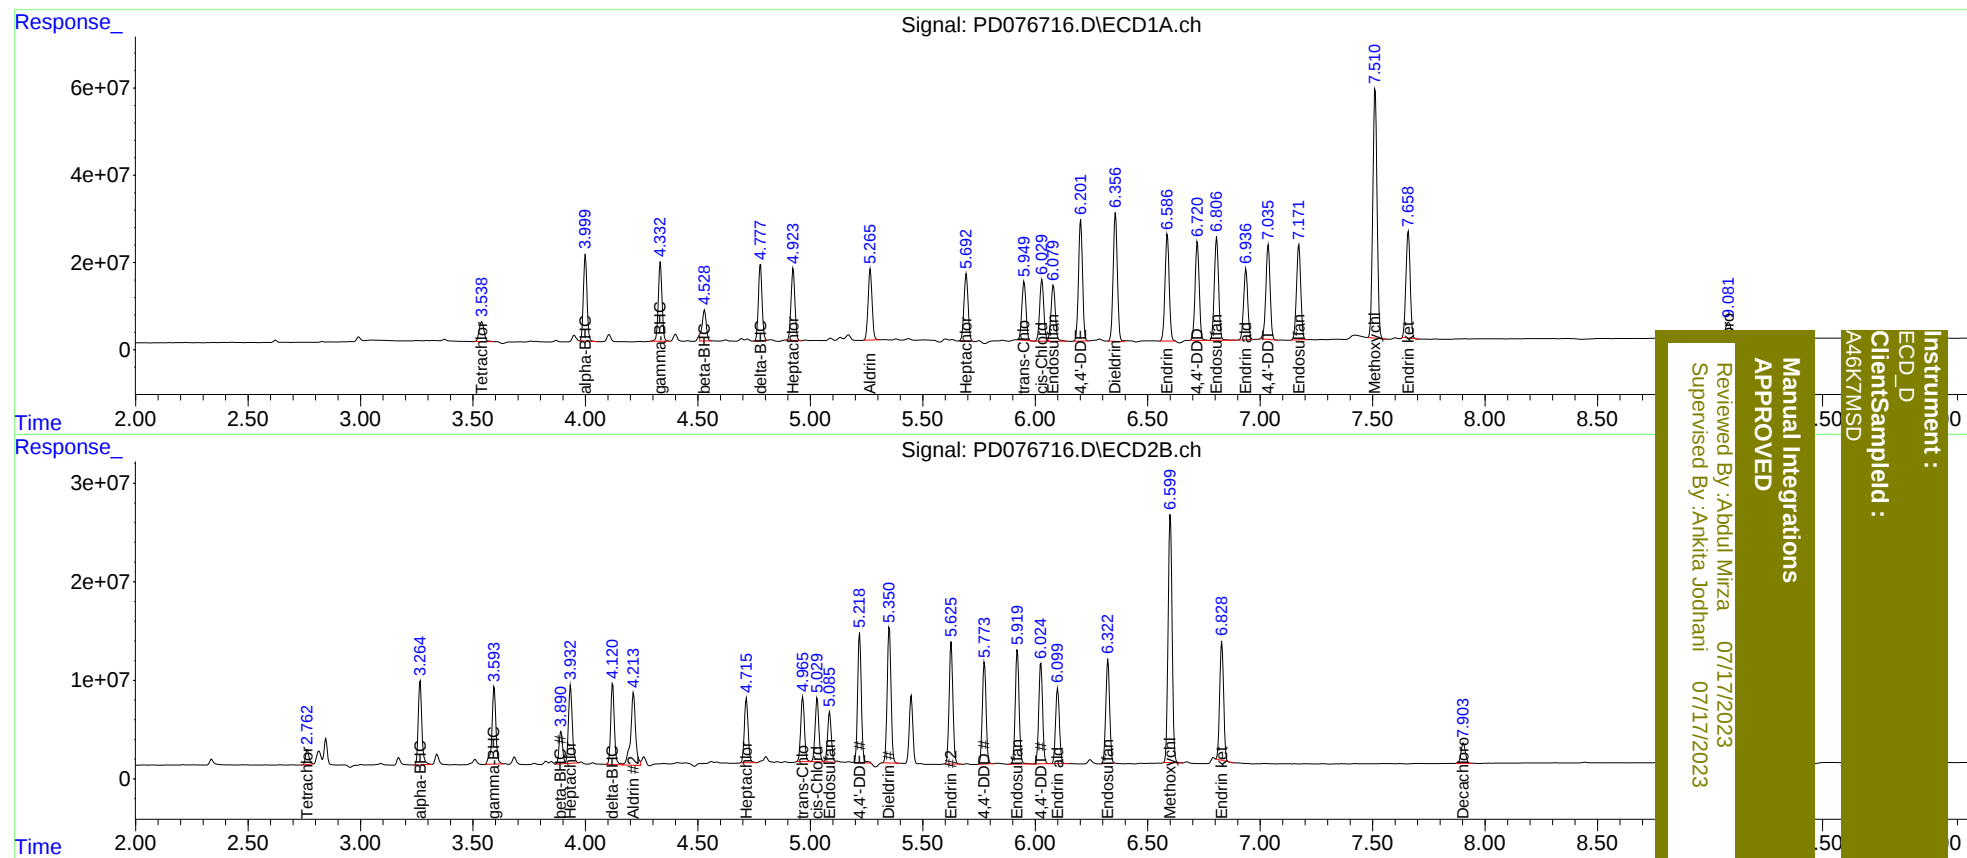

Instrument :
ECD_D
ClientSampled :
A46K7MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023