

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
 Data File : PD076733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 05:12
 Operator : AR\AJ
 Sample : 03444-09MSD
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46Q1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 06:52:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.764	296.9E6	13830454	139.571m	12.957 #
27)	SA Decachlor...	9.084	7.904	70089493	29317886	28.849	27.349
Target Compounds							
2)	A alpha-BHC	4.000	3.266	191.5E6	78460084	54.042m	49.584
3)	MA gamma-BHC...	4.335	3.593	334.8E6	78546950	100.944m	52.430m#
4)	MA Heptachlor	4.924	3.934	172.7E6	169.6E6	49.672m	113.403 #
5)	MB Aldrin	5.268	4.216	171.4E6	85056783	50.124	56.517m
6)	B beta-BHC	4.526	3.892	51189061	27063565	33.678m	37.778
7)	B delta-BHC	4.780	4.122	212.8E6	88490610	63.465m	57.977
8)	B Heptachlo...	5.694	4.716	176.9E6	78392672	59.054	55.721
9)	A Endosulfan I	6.082	5.086	141.2E6	52057176	49.579	42.016
10)	B trans-Chl...	5.951	4.966	160.6E6	80511513	52.223m	59.540m
11)	B cis-Chlor...	6.032	5.030	157.3E6	64393961	49.627	45.643
12)	B 4,4'-DDE	6.204	5.220	304.3E6	127.0E6	104.433	105.116
13)	MA Dieldrin	6.358	5.352	335.8E6	171.3E6	106.438	122.835
14)	MA Endrin	6.589	5.628	276.9E6	124.3E6	107.428	100.499
15)	B Endosulfa...	6.808	5.921	260.8E6	118.0E6	98.106	98.116
16)	A 4,4'-DDD	6.722	5.775	256.0E6	103.1E6	113.299	108.772
17)	MA 4,4'-DDT	7.036	6.026	243.3E6	112.3E6	108.954m	119.856
18)	B Endrin al...	6.938	6.100	177.9E6	81574801	95.124	97.251m
19)	B Endosulfa...	7.173	6.324	246.0E6	111.4E6	98.514	99.888
20)	A Methoxychlor	7.513	6.600	662.4E6	282.2E6	500.425	528.882m
21)	B Endrin ke...	7.658	6.831	262.1E6	128.7E6	94.652m	100.594

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071423\
Data File : PD076733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 05:12
Operator : AR\AJ
Sample : 03444-09MSD
Misc :
ALS Vial : 71 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 06:52:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

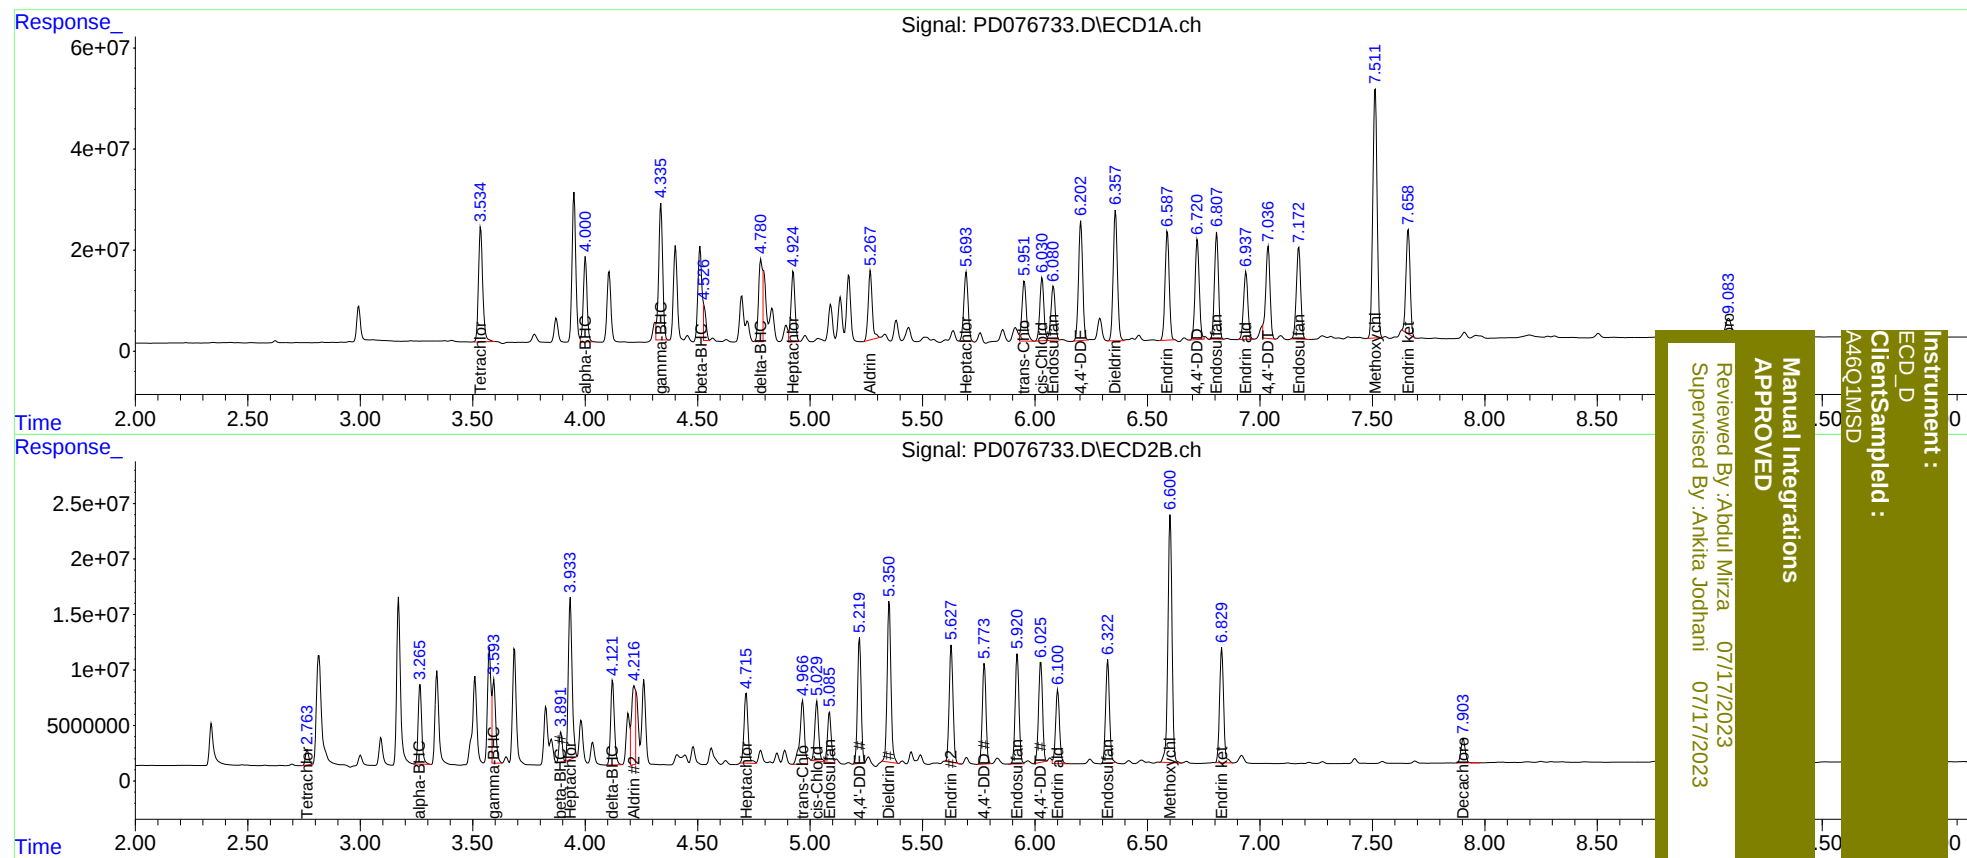

Instrument :
ECD_D
ClientSampled :
A46Q1MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023