

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071521\
Data File : PD064289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 18:49
Operator : AR\AJ
Sample : M3008-01
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
BGE65

Manual Integrations
APPROVED

mohammad
7/16/2021 9:11:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 05:33:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

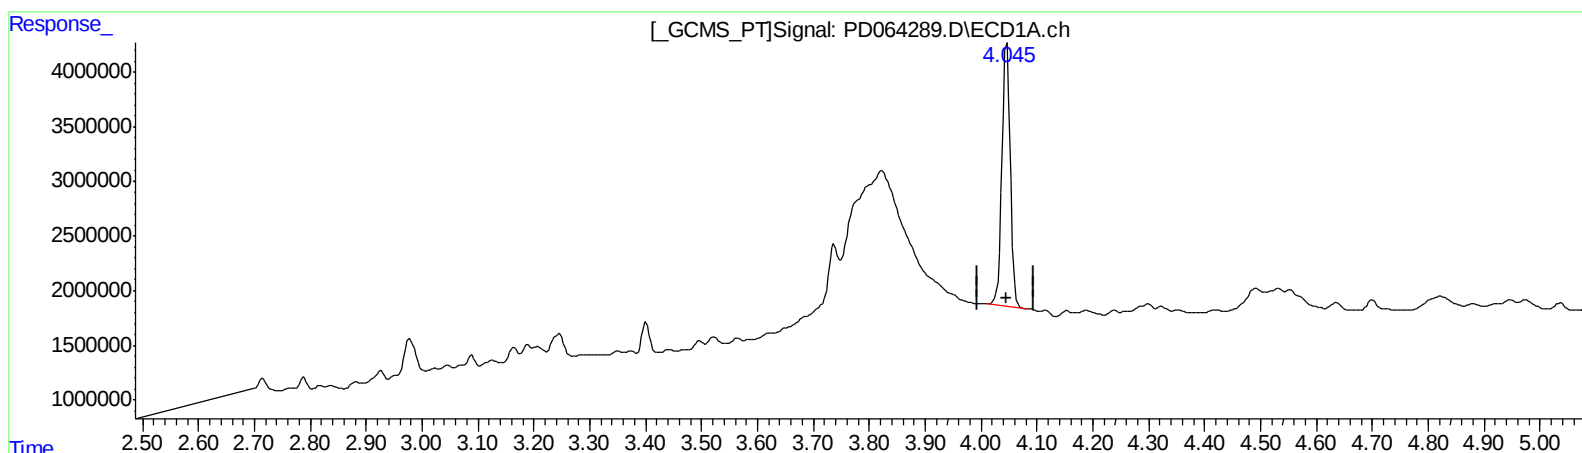

(1) Tetrachloro-m-xylene (SA)

4.046min 18.427 ng/ml

response 24655400

(1) Tetrachloro-m-xylene #2 (SA)

3.512min 19.259 ng/ml

response 192420860

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071521\
Data File : PD064289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 18:49
Operator : AR\AJ
Sample : M3008-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BGE65

Manual Integrations
APPROVED

mohammad
7/16/2021 9:11:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 05:33:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.046	3.511	24655400	203.3E6	18.427	20.344m
27)	SA Decachlor...	9.209	8.255	48427799	208.9E6	45.155	39.993

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

> AJ
07/20/21