

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
 Data File : PD076769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 13:27
 Operator : AR\AJ
 Sample : 03452-22MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46Q0MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 23:58:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.764	28385710	7056609	13.343	6.611 #
27)	SA Decachlor...	9.084	7.904	26956329	12042187	11.095	11.234
Target Compounds							
2)	A alpha-BHC	4.001	3.266	222.4E6	94765649	62.740	59.889
3)	MA gamma-BHC...	4.334	3.595	201.2E6	84017148	60.643	56.081
4)	MA Heptachlor	4.925	3.934	199.6E6	88914828	57.415	59.467
5)	MB Aldrin	5.268	4.214	202.7E6	99150951	59.286	65.882
6)	B beta-BHC	4.529	3.892	83786637	36549394	55.124m	51.020
7)	B delta-BHC	4.779	4.122	202.6E6	90584570	60.422	59.349
8)	B Heptachlo...	5.695	4.716	175.9E6	78065108	58.695	55.489
9)	A Endosulfan I	6.082	5.087	166.9E6	72108102	58.603	58.199
10)	B trans-Chl...	5.952	4.967	173.3E6	77703450	56.359	57.463
11)	B cis-Chlor...	6.031	5.031	182.0E6	78001333	57.407	55.288
12)	B 4,4'-DDE	6.203	5.219	347.1E6	152.3E6	119.140	126.021
13)	MA Dieldrin	6.358	5.351	374.4E6	164.4E6	118.671	117.873
14)	MA Endrin	6.588	5.627	312.3E6	146.1E6	121.167	118.156
15)	B Endosulfa...	6.809	5.921	310.0E6	139.2E6	116.611	115.775
16)	A 4,4'-DDD	6.721	5.774	289.7E6	126.3E6	128.206	133.277
17)	MA 4,4'-DDT	7.037	6.026	279.4E6	120.9E6	125.157	129.058
18)	B Endrin al...	6.938	6.101	201.3E6	90005688	107.635	107.302
19)	B Endosulfa...	7.173	6.324	283.7E6	127.0E6	113.595	113.864
20)	A Methoxychlor	7.513	6.601	746.1E6	311.2E6	563.646	583.067
21)	B Endrin ke...	7.658	6.828	332.0E6	148.0E6	119.920m	115.636m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:27
Operator : AR\AJ
Sample : 03452-22MS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 23:58:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

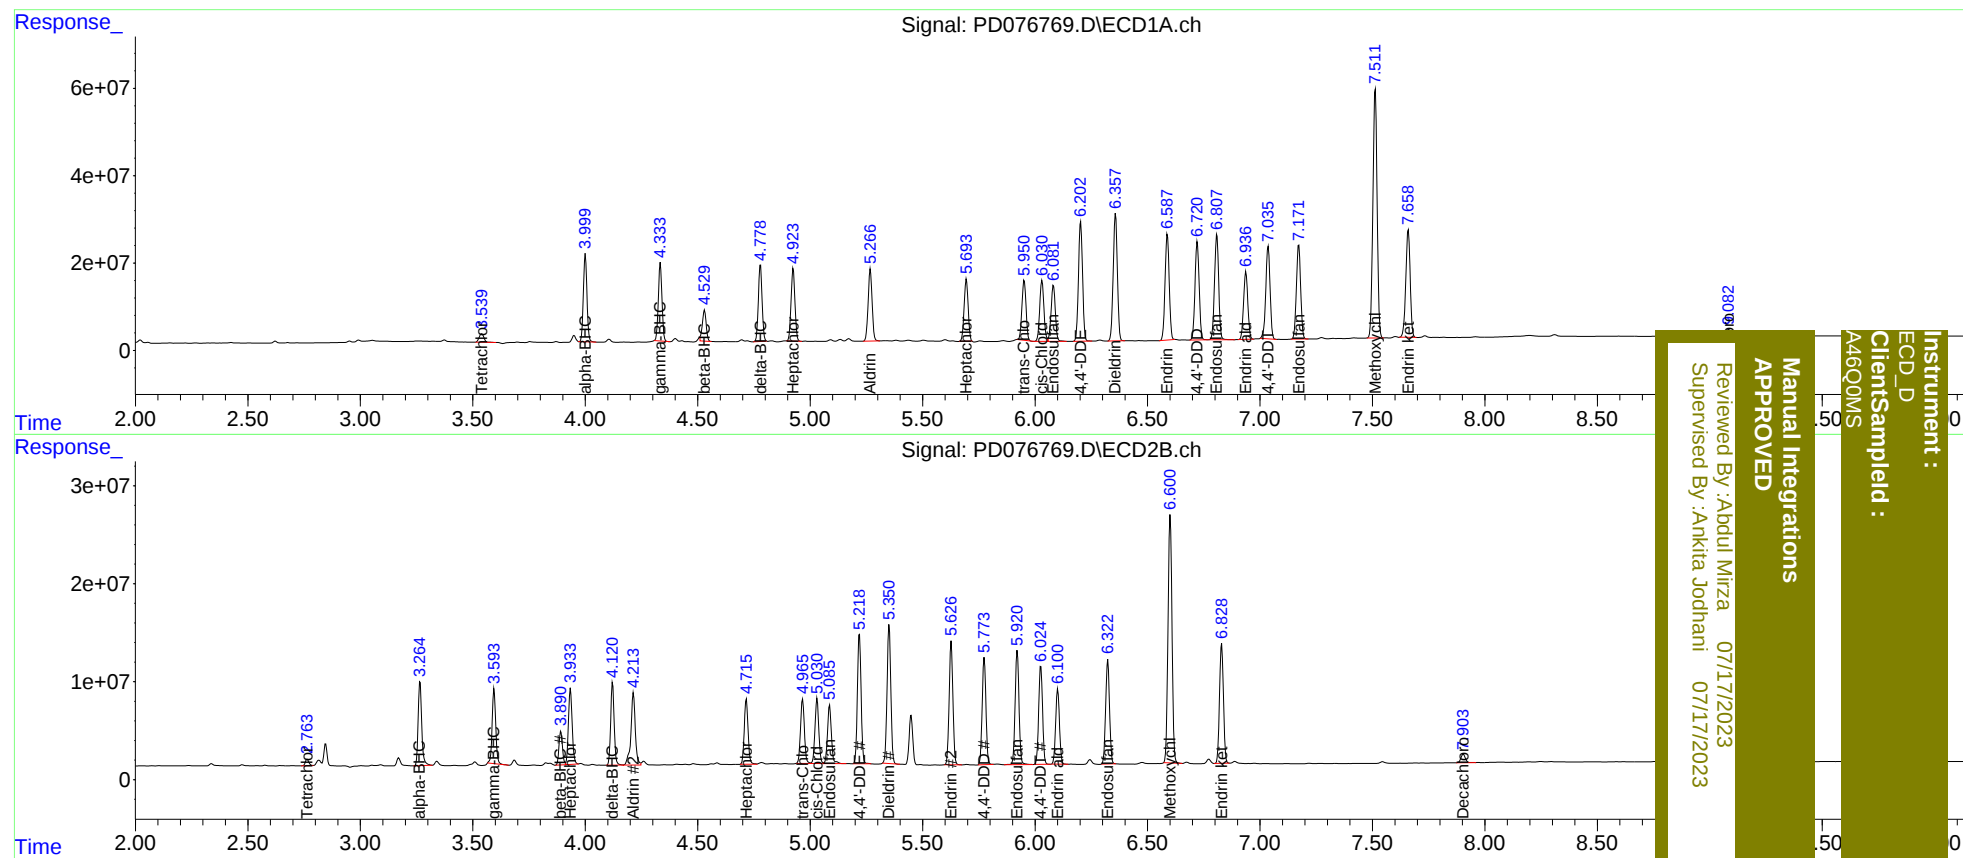

Instrument :
ECD_D
ClientSampled :
A46Q0MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023