

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
 Data File : PD076770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 13:40
 Operator : AR\AJ
 Sample : 03452-23MSD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46Q0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 23:58:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.764	28999189	7188788	13.632	6.735 #
27)	SA Decachlor...	9.085	7.905	27303548	12139531	11.238	11.324
Target Compounds							
2)	A alpha-BHC	4.001	3.266	220.5E6	94321092	62.221	59.608
3)	MA gamma-BHC...	4.335	3.595	199.5E6	85098240	60.150	56.803
4)	MA Heptachlor	4.925	3.935	197.1E6	89032900	56.707	59.546
5)	MB Aldrin	5.268	4.215	200.1E6	100.8E6	58.517	66.987
6)	B beta-BHC	4.530	3.893	85748869	36459323	56.415m	50.894
7)	B delta-BHC	4.780	4.122	200.2E6	90276056	59.696	59.147
8)	B Heptachlo...	5.695	4.718	174.6E6	77948157	58.284	55.405
9)	A Endosulfan I	6.082	5.088	166.4E6	72162739	58.407	58.243
10)	B trans-Chl...	5.952	4.967	171.8E6	78288017	55.884	57.895
11)	B cis-Chlor...	6.031	5.032	181.3E6	78480673	57.195	55.627
12)	B 4,4'-DDE	6.204	5.220	344.8E6	152.7E6	118.361	126.371
13)	MA Dieldrin	6.358	5.352	372.7E6	165.2E6	118.122	118.499
14)	MA Endrin	6.589	5.627	309.7E6	146.6E6	120.127	118.513
15)	B Endosulfa...	6.808	5.921	306.8E6	139.6E6	115.405	116.112
16)	A 4,4'-DDD	6.722	5.775	287.4E6	127.0E6	127.204	133.983
17)	MA 4,4'-DDT	7.038	6.026	276.2E6	121.8E6	123.721	129.983
18)	B Endrin al...	6.938	6.101	199.3E6	90863273	106.564	108.324
19)	B Endosulfa...	7.174	6.324	280.5E6	127.9E6	112.311	114.638
20)	A Methoxychlor	7.513	6.602	739.3E6	313.4E6	558.494	587.172
21)	B Endrin ke...	7.660	6.830	319.2E6	148.2E6	115.303	115.850

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:40
Operator : AR\AJ
Sample : 03452-23MSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 23:58:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

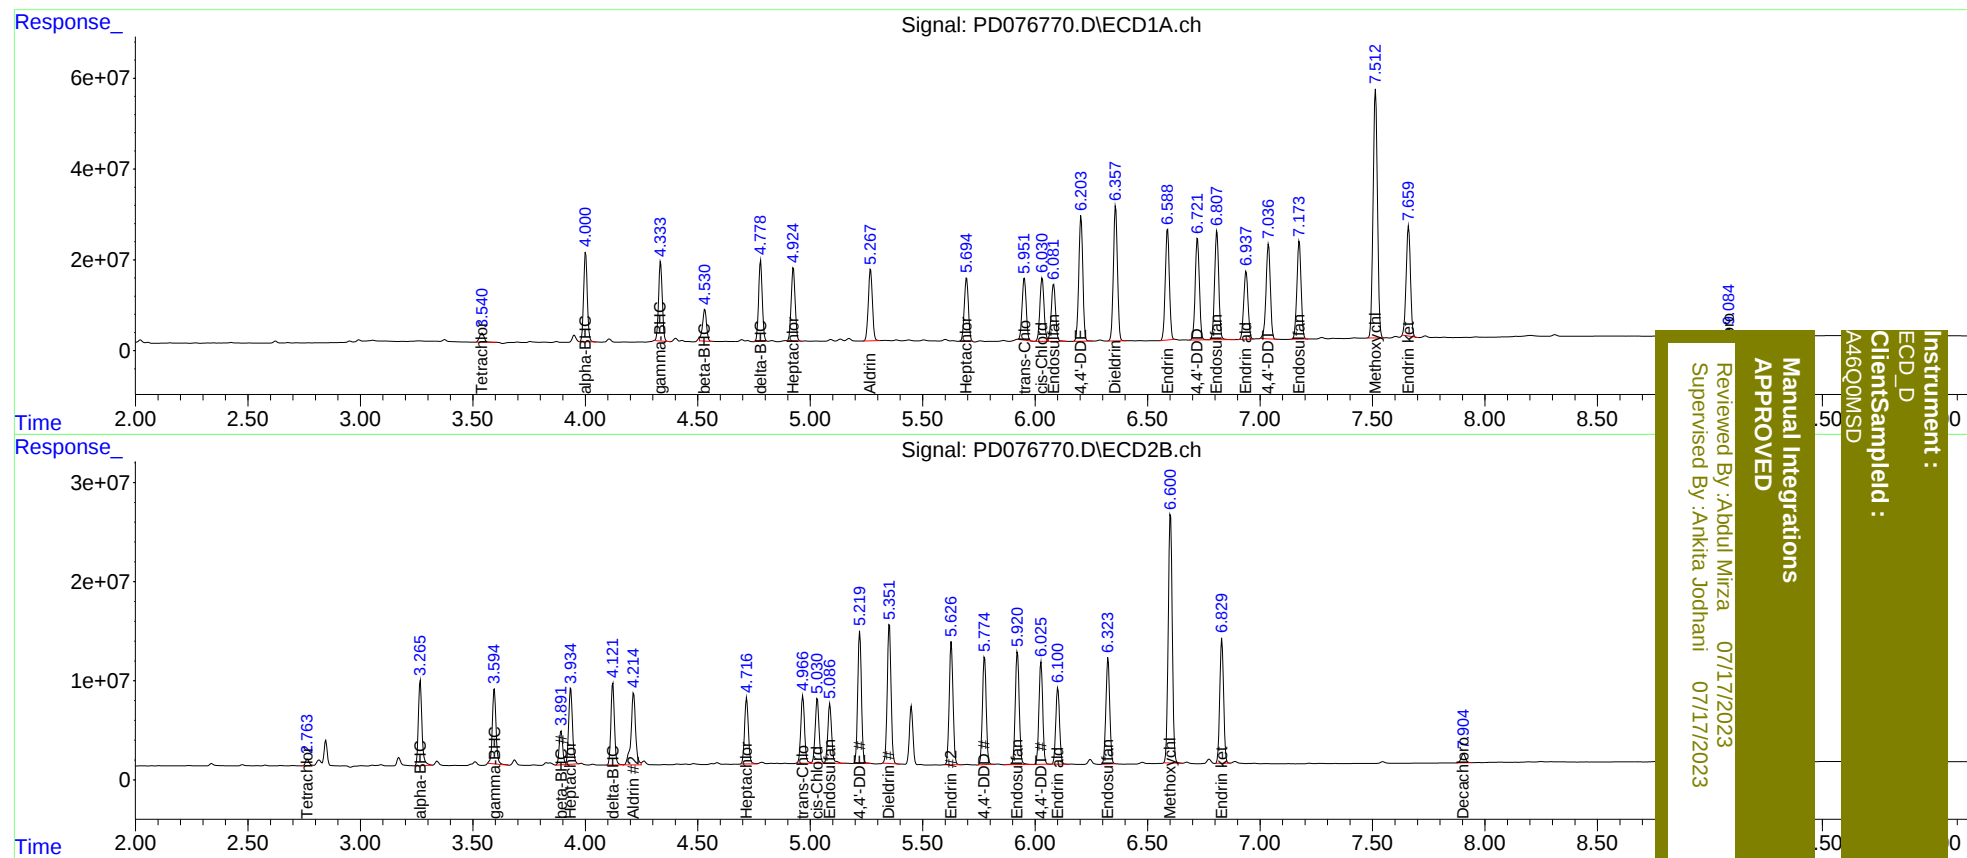

Instrument :
ECD_D
ClientSampled :
A46Q0MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023