

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
 Data File : PD076779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 16:08
 Operator : AR\AJ
 Sample : 03458-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46M1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 00:01:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.764	31102817	13884361	14.620	13.007
2)	SA Decachlor...	9.083	7.904	57744647	24779211	23.768	23.115
Target Compounds							
3)	MA gamma-BHC...	4.337	3.572	12067041	3674485	3.638m	2.453m#
7)	B delta-BHC	4.795	4.130	9690746	2722422	2.890m	1.784 #
17)	MA 4,4'-DDT	7.007	6.020	2252065	1686339	1.009m	1.800 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 16:08
Operator : AR\AJ
Sample : 03458-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 00:01:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

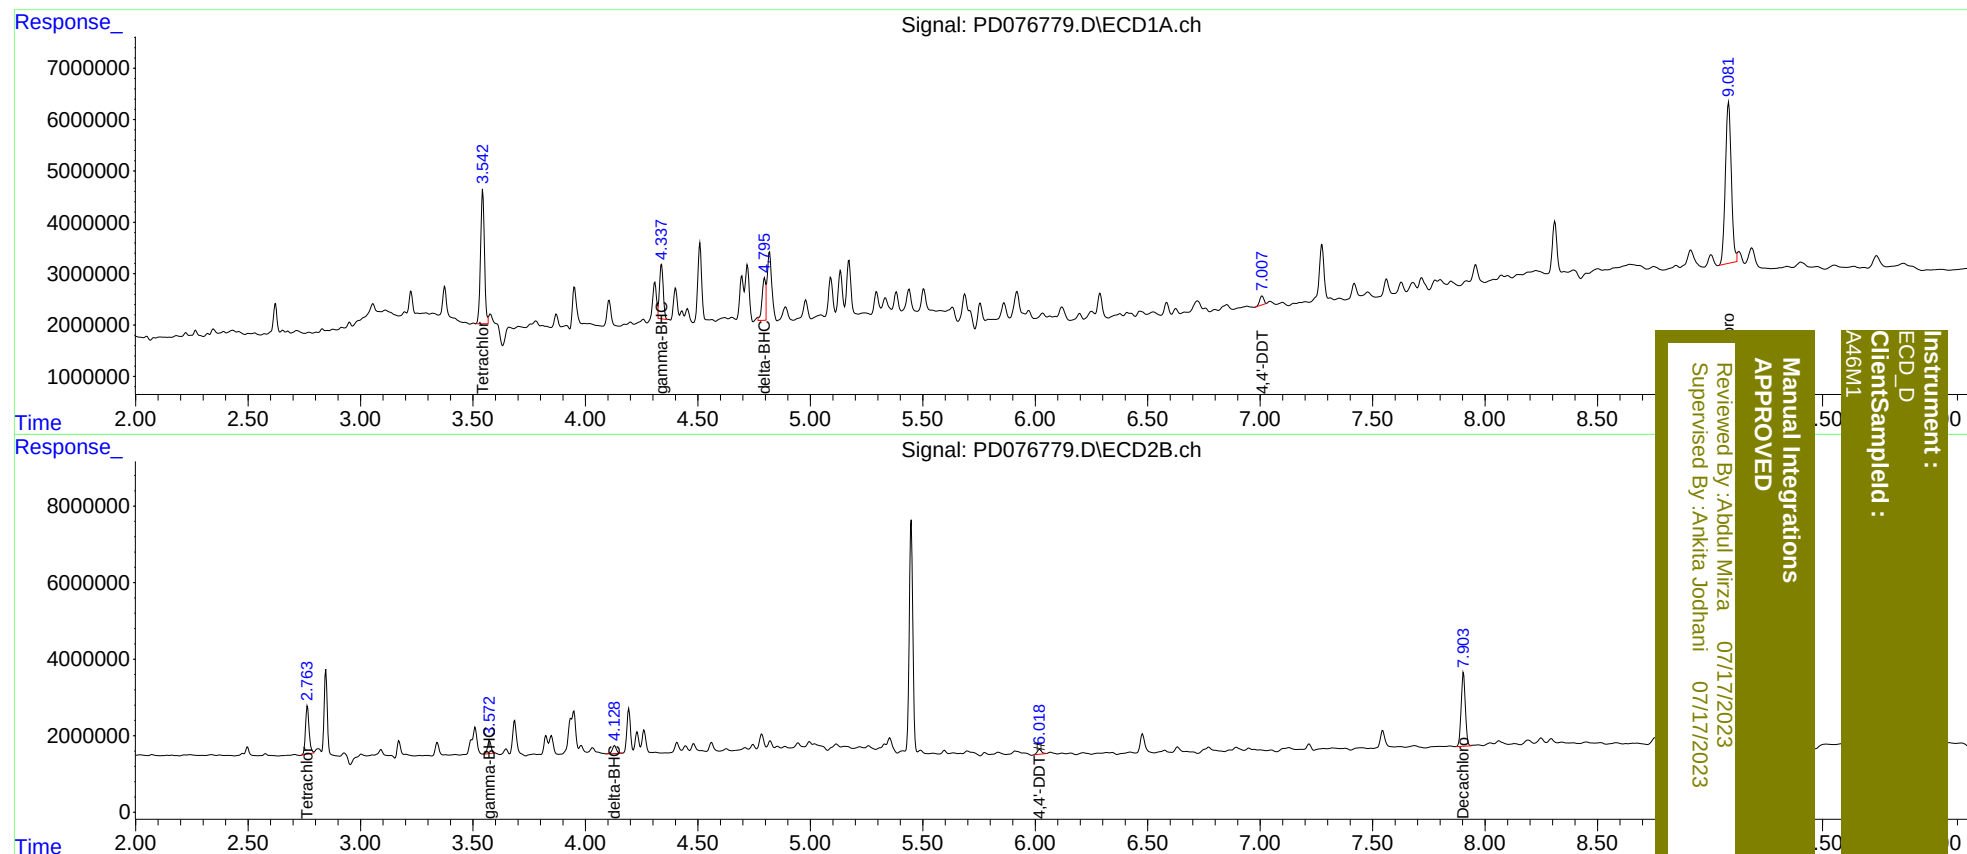

Instrument :
ECD_D
ClientSampled :
A46M1

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023