

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:13
Operator : AR\AJ
Sample : 03452-21
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
A46Q0

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 09:27:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

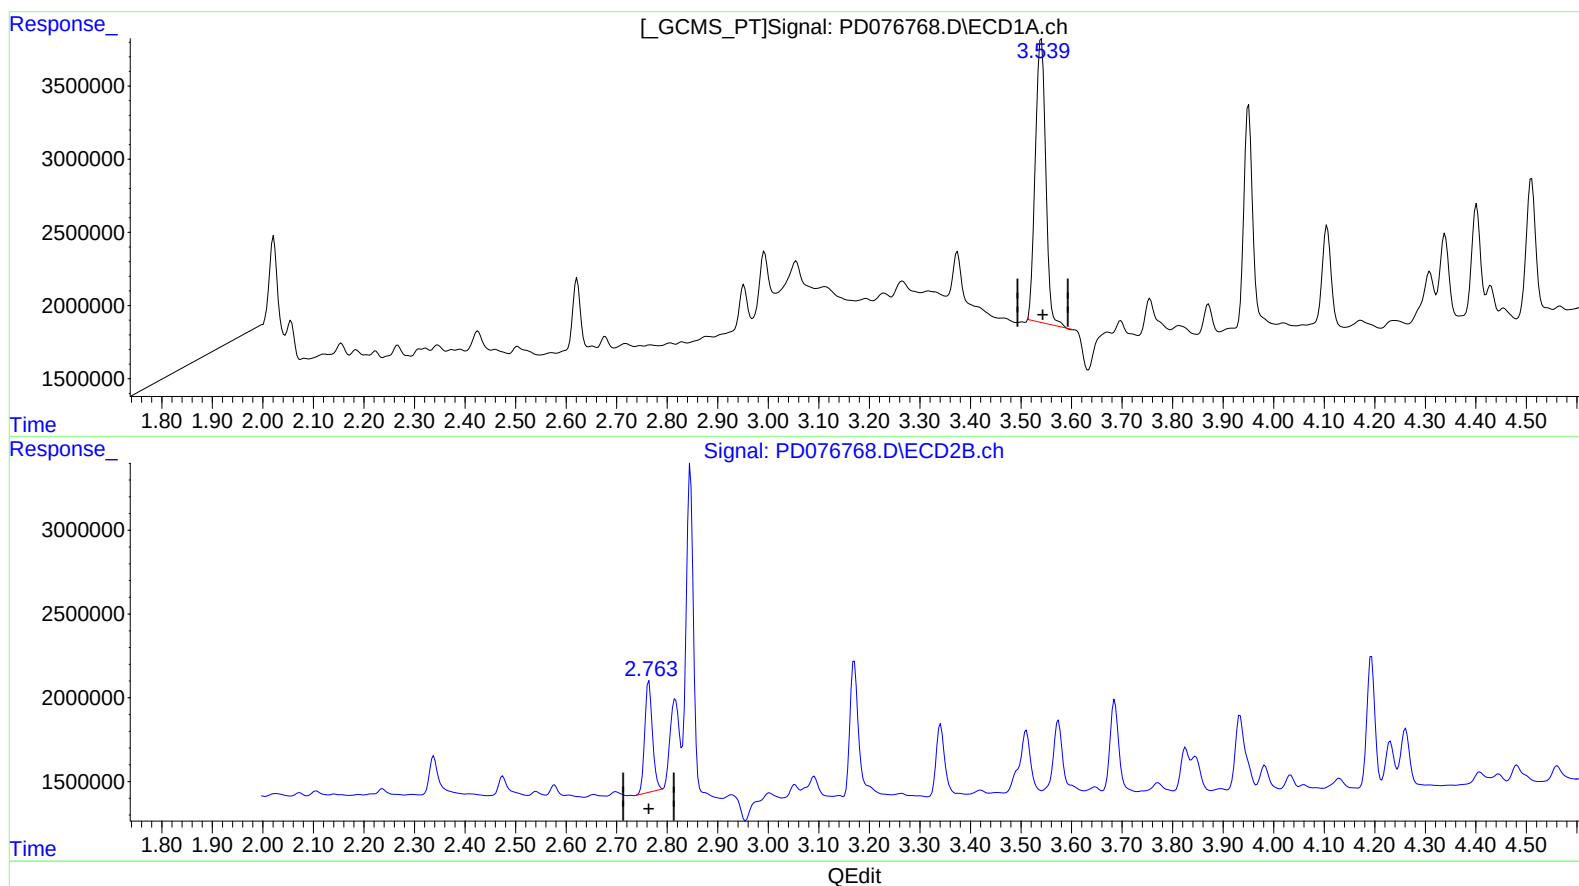

(1) Tetrachloro-m-xylene (SA)

3.540min 13.089 ng/ml

response 27844301

(1) Tetrachloro-m-xylene #2 (SA)

2.764min 6.588 ng/ml

response 7031622

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:13
Operator : AR\AJ
Sample : 03452-21
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
A46Q0

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 23:57:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

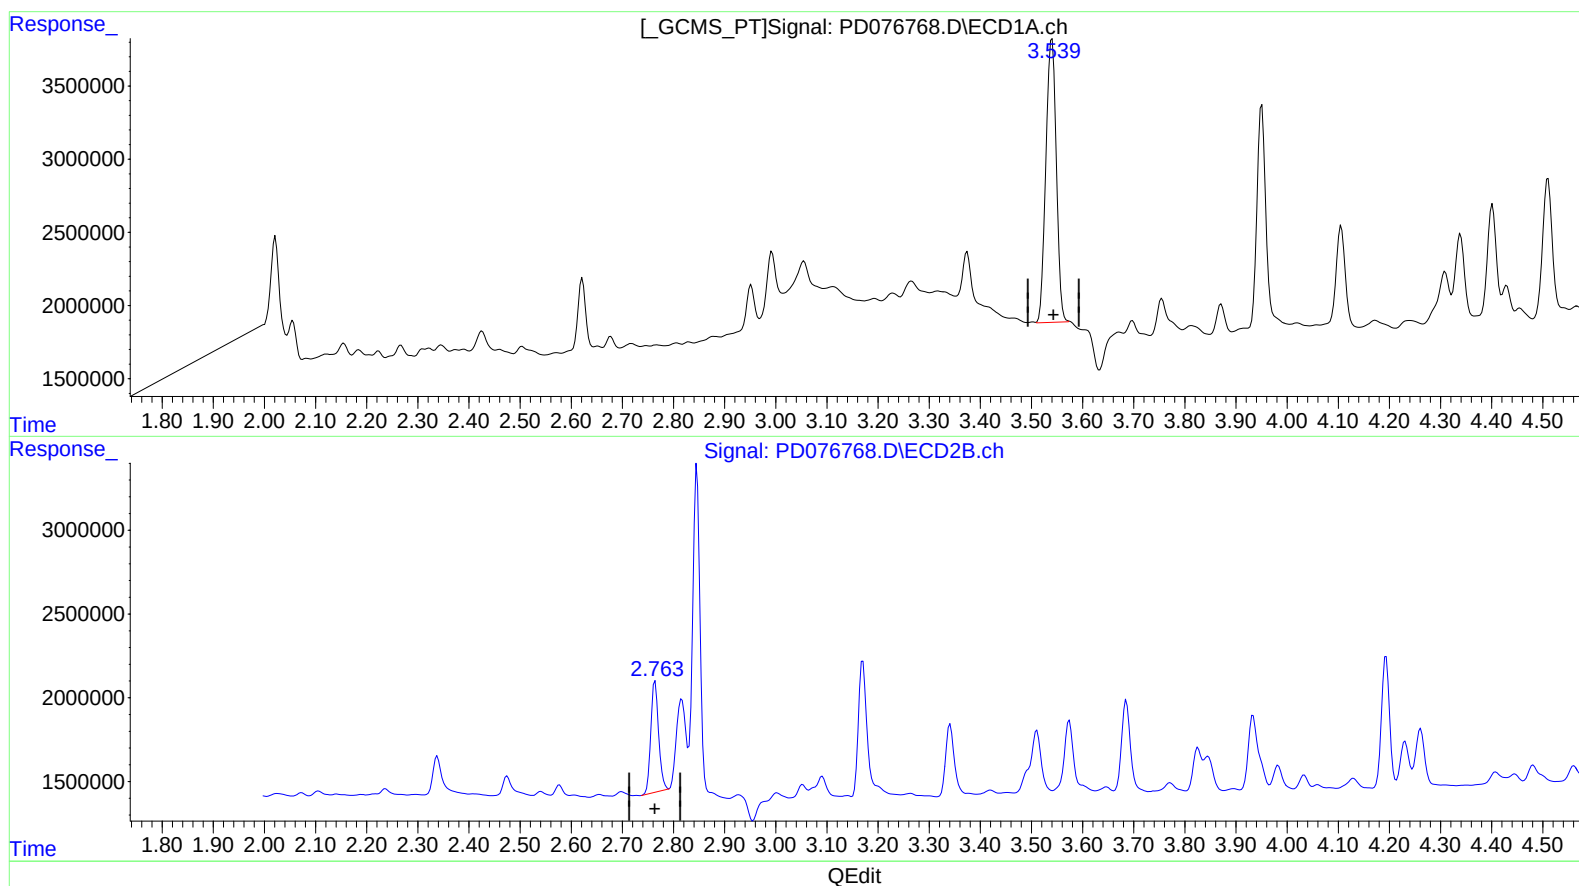

(1) Tetrachloro-m-xylene (SA)

3.539min 12.976 ng/ml m

response 27604860

(1) Tetrachloro-m-xylene #2 (SA)

2.764min 6.588 ng/ml

response 7031622

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:13
Operator : AR\AJ
Sample : 03452-21
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
A46Q0

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 09:27:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

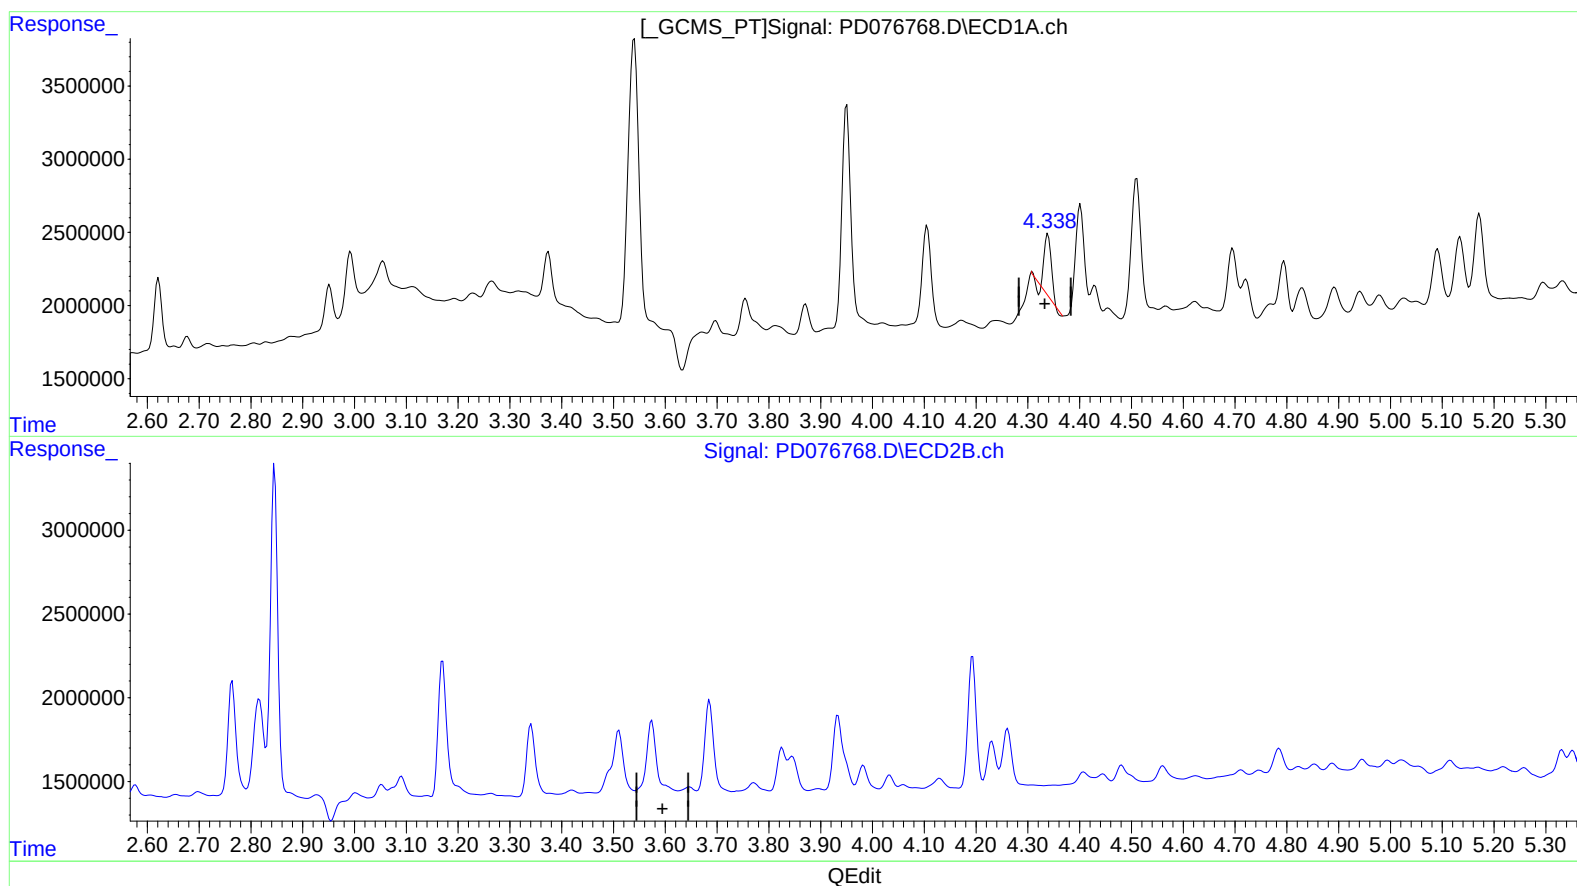

(3) gamma-BHC (Lindane) (MA)

4.339min 1.126 ng/ml

response 3734432

(3) gamma-BHC (Lindane) #2 (MA)

3.574min -0.138 ng/ml

response -206180

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:13
Operator : AR\AJ
Sample : 03452-21
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
A46Q0

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 23:57:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

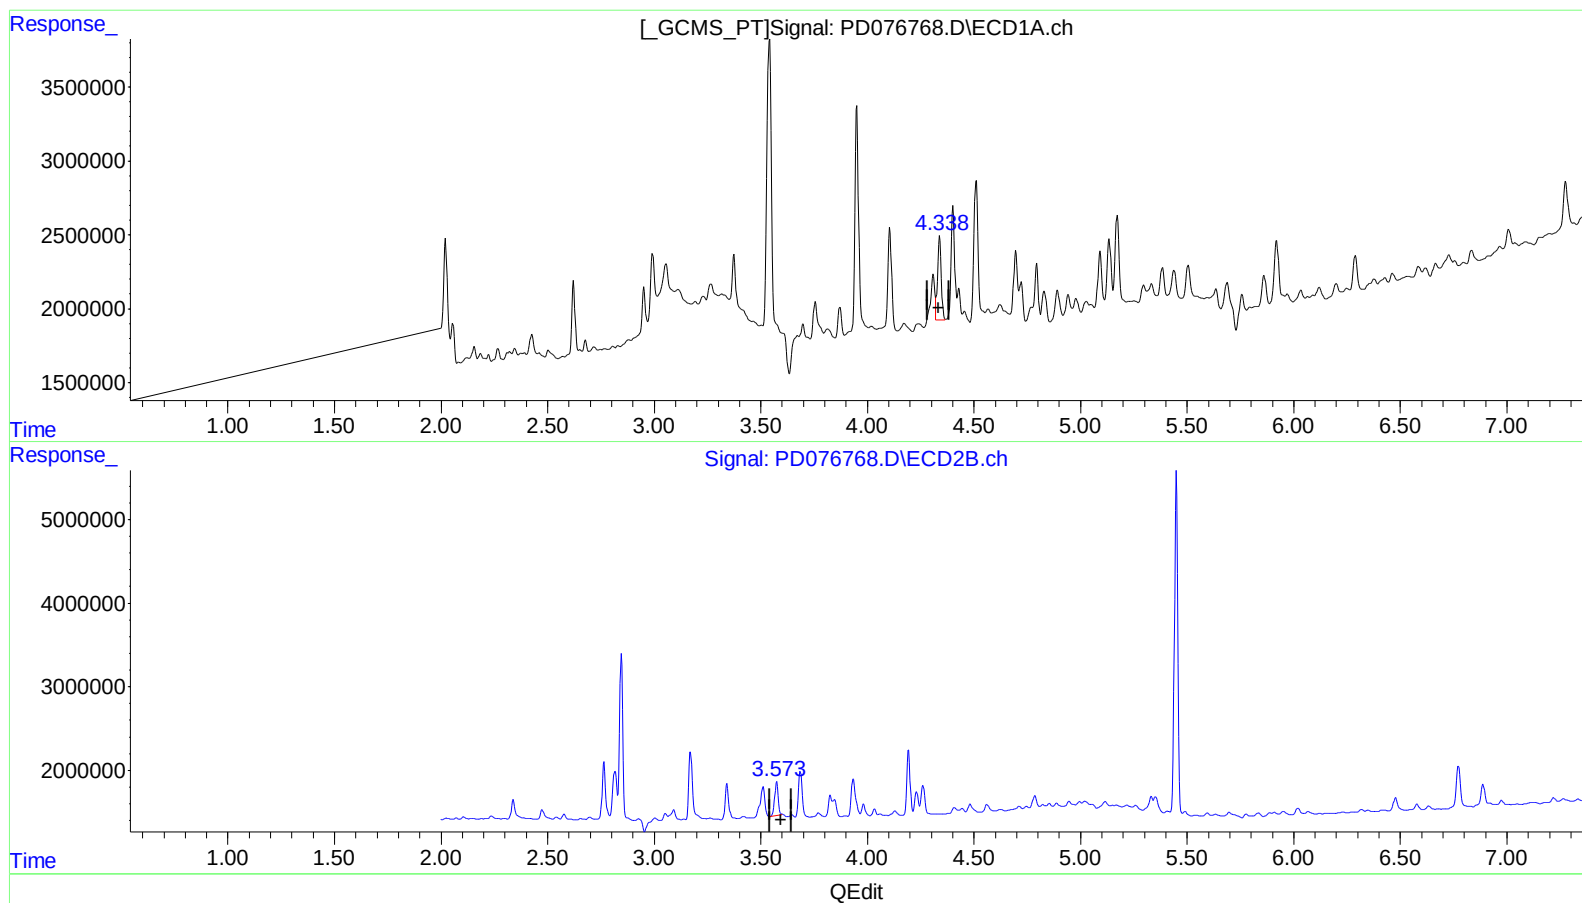

(3) gamma-BHC (Lindane) (MA)

4.338min 2.124 ng/ml m

response 7044783

(3) gamma-BHC (Lindane) #2 (MA)

3.573min 3.068 ng/ml m

response 4596294

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:13
Operator : AR\AJ
Sample : 03452-21
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
A46Q0

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 23:57:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

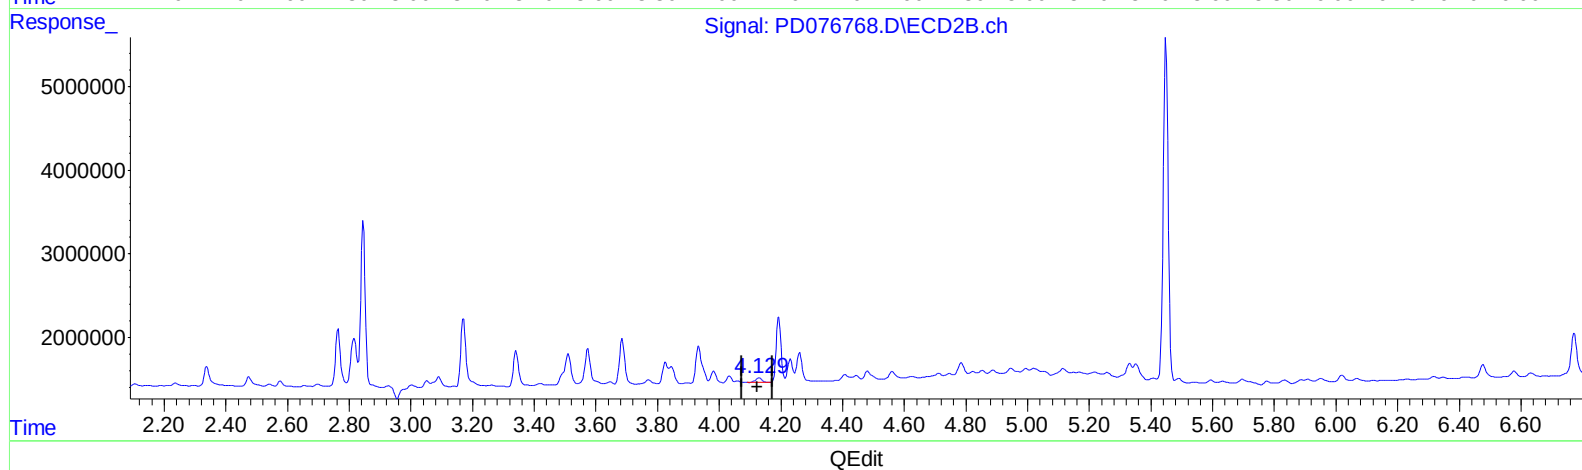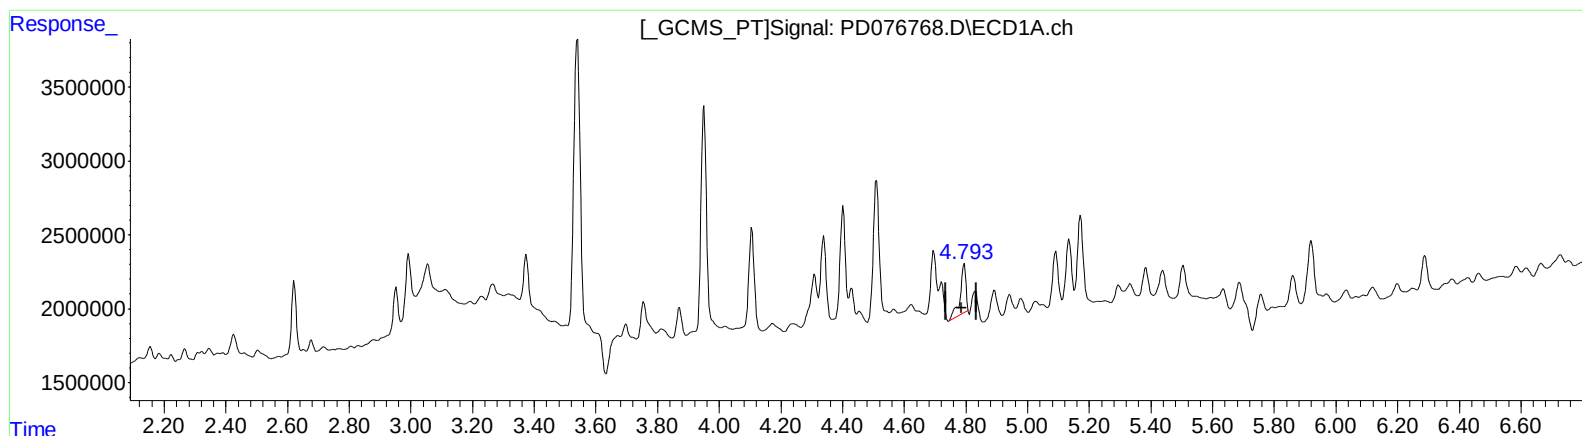

(7) delta-BHC (B)

4.795min 1.300 ng/ml

response 4358885

(7) delta-BHC #2 (B)

4.130min 0.518 ng/ml

response 790877

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:13
Operator : AR\AJ
Sample : 03452-21
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
A46Q0

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 23:57:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

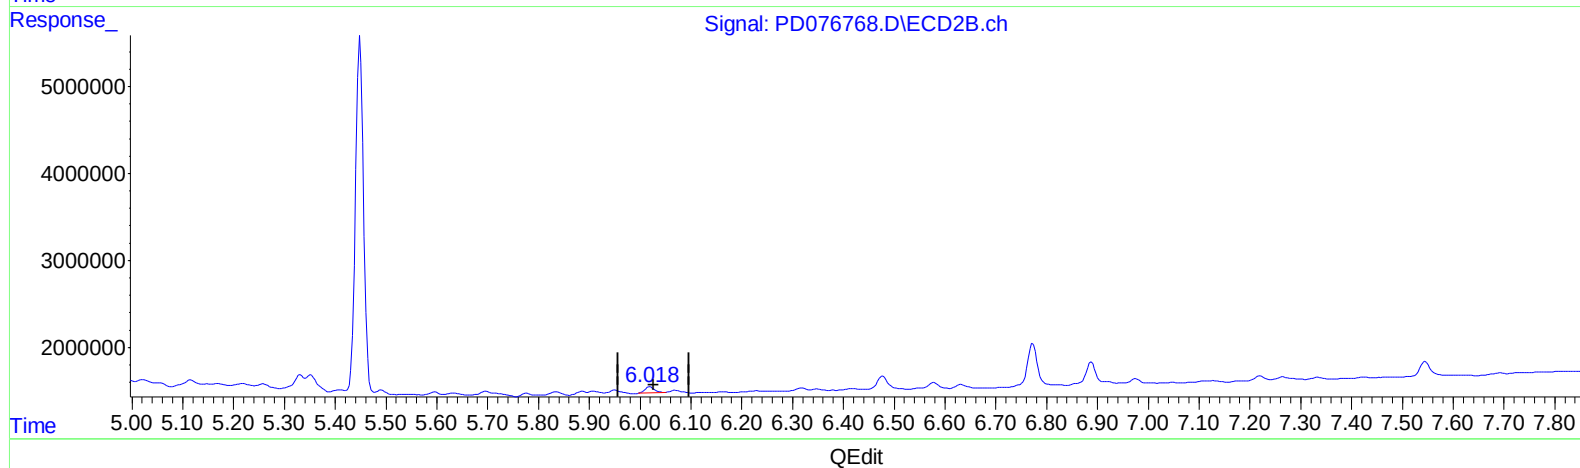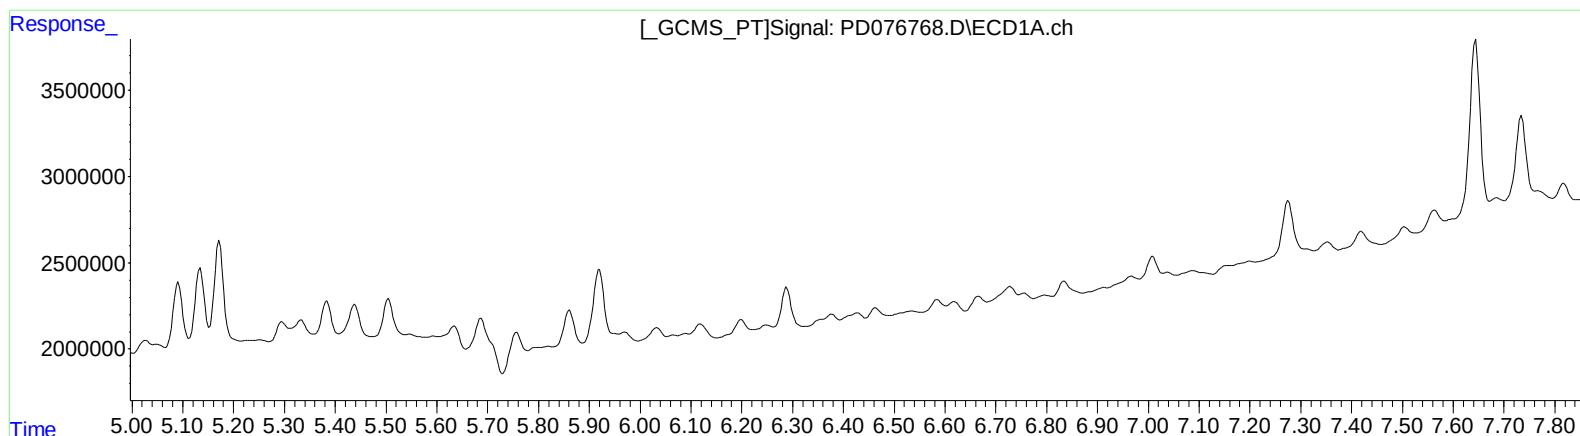

(17) 4,4'-DDT (MA)

0.000min 0.000 ng/ml

response 0

(17) 4,4'-DDT #2 (MA)

6.020min 0.993 ng/ml

response 929774

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 13:13
Operator : AR\AJ
Sample : 03452-21
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
A46Q0

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 23:57:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

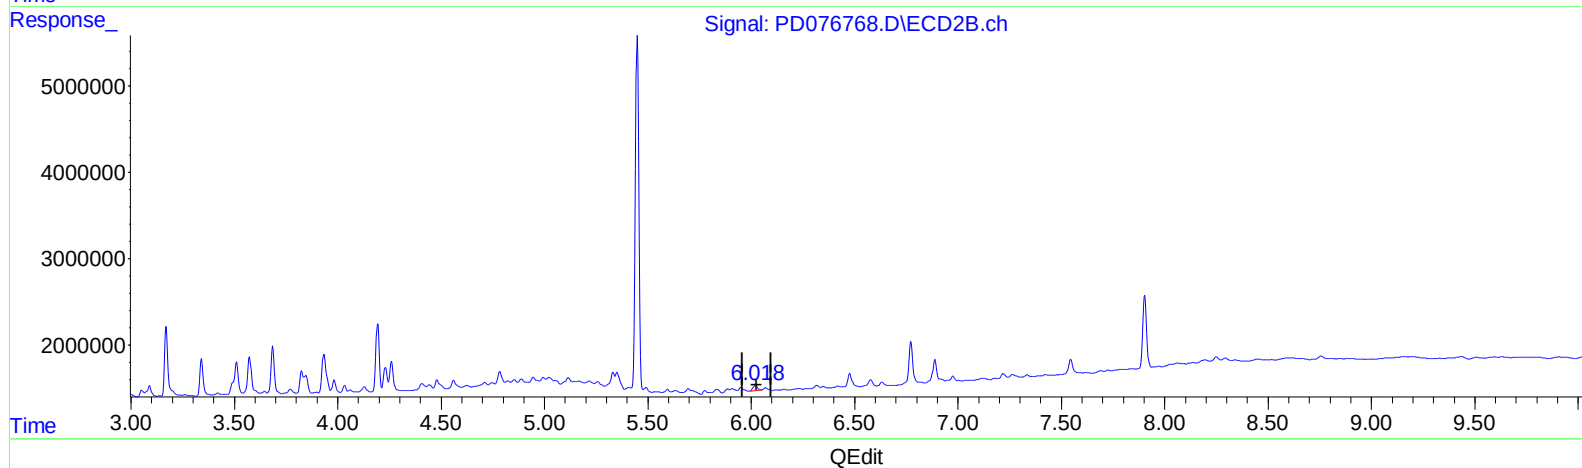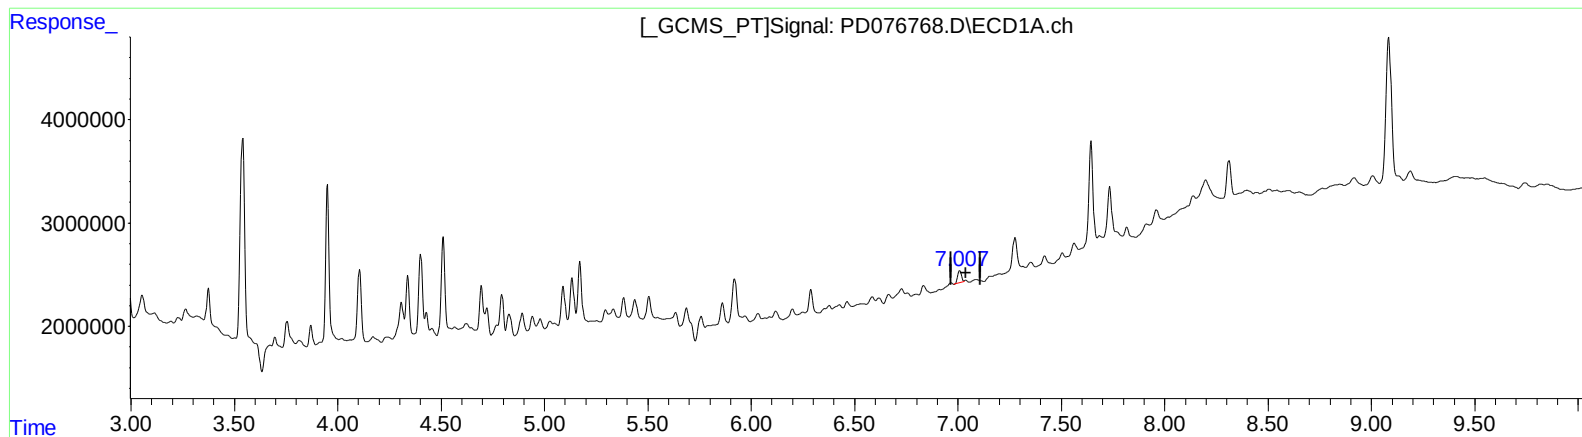

(17) 4,4'-DDT (MA)

7.007min 0.617 ng/ml m

response 1377630

(17) 4,4'-DDT #2 (MA)

6.020min 0.993 ng/ml

response 929774