

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 16:21
Operator : AR\AJ
Sample : 03458-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
A46M2



Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 00:01:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

07/17/2023
Supervised By :Ankita
Jodhani

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

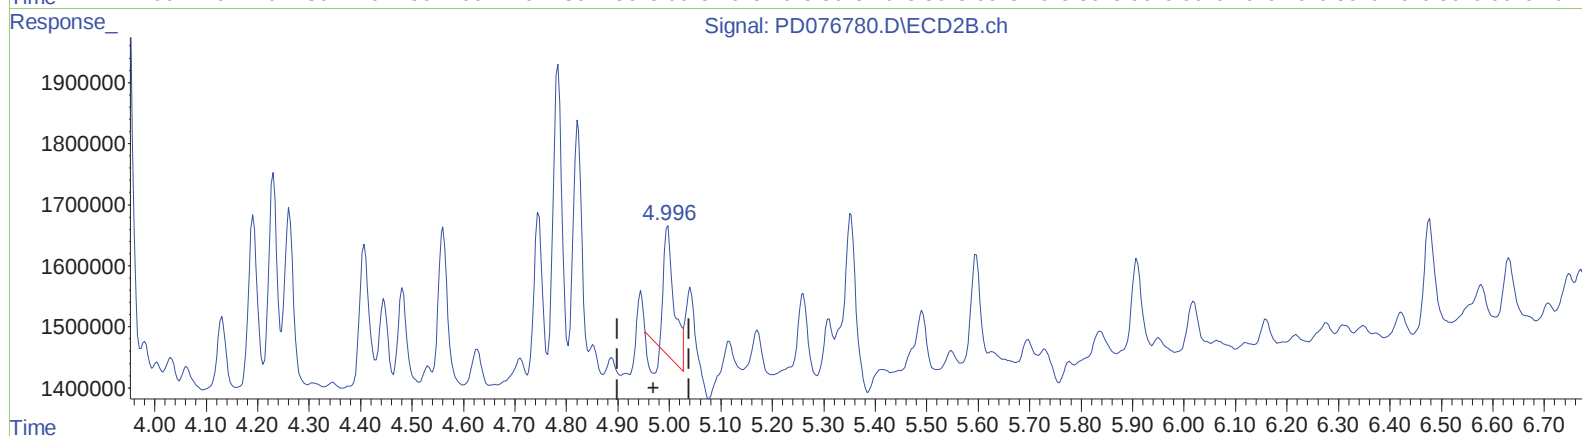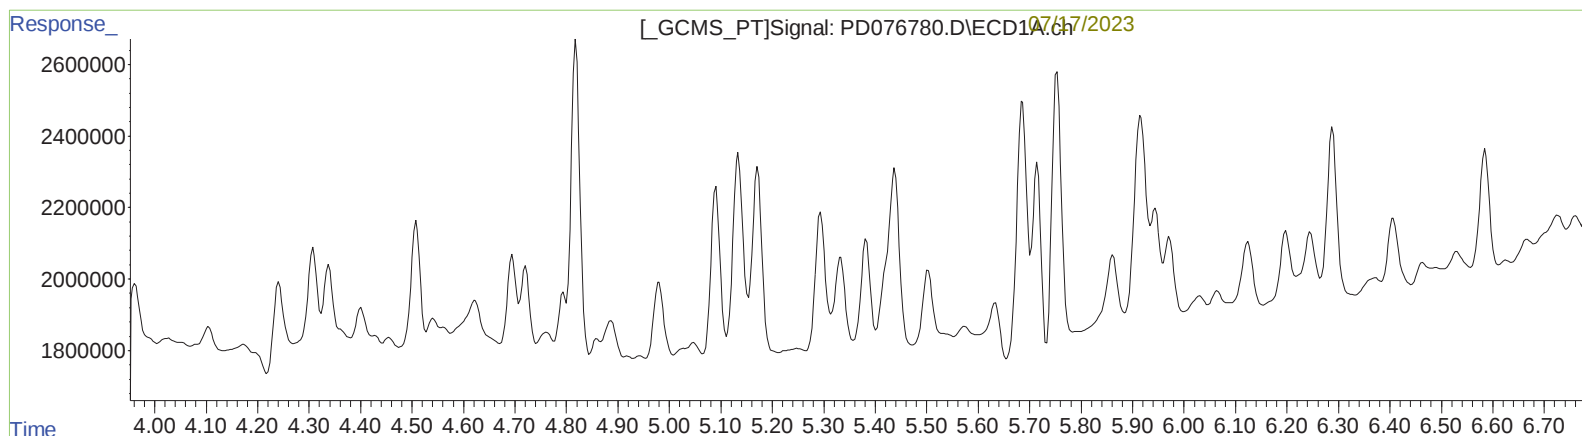

QEdit

(10) trans-Chlordane (B)
0.000min 0.000 ng/ml
response 0

(10) trans-Chlordane #2 (B)
4.997min 1.879 ng/ml
response 2540800

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
 Data File : PD076780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 16:21
 Operator : AR\AJ
 Sample : 03458-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46M2



Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 00:01:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

07/17/2023
 Supervised By :Ankita
 Jodhani

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

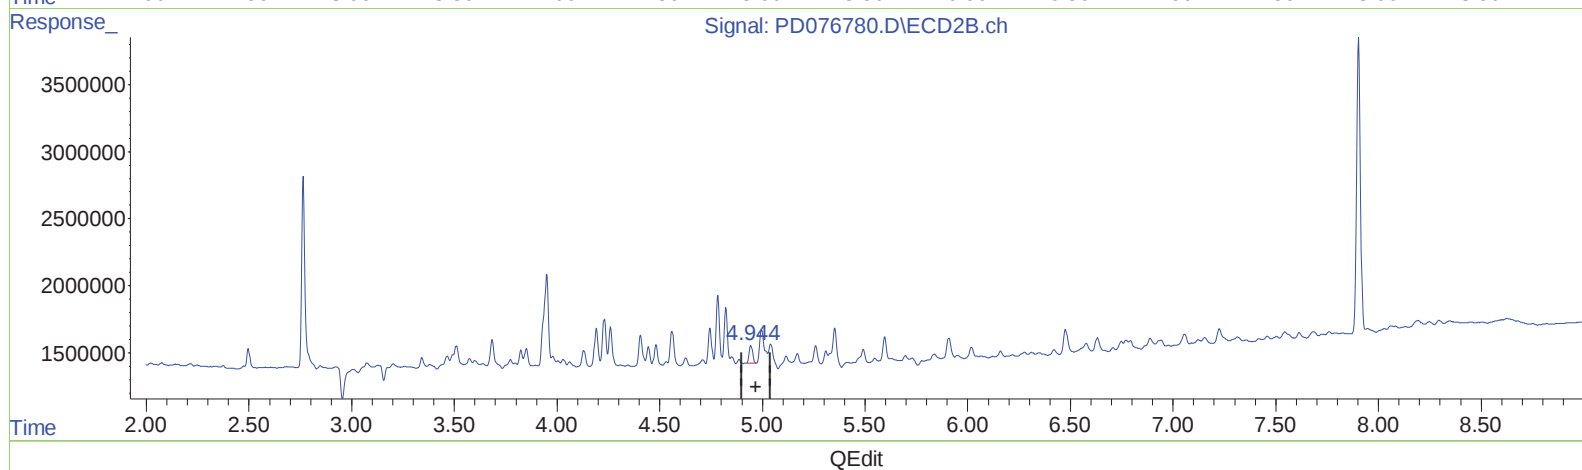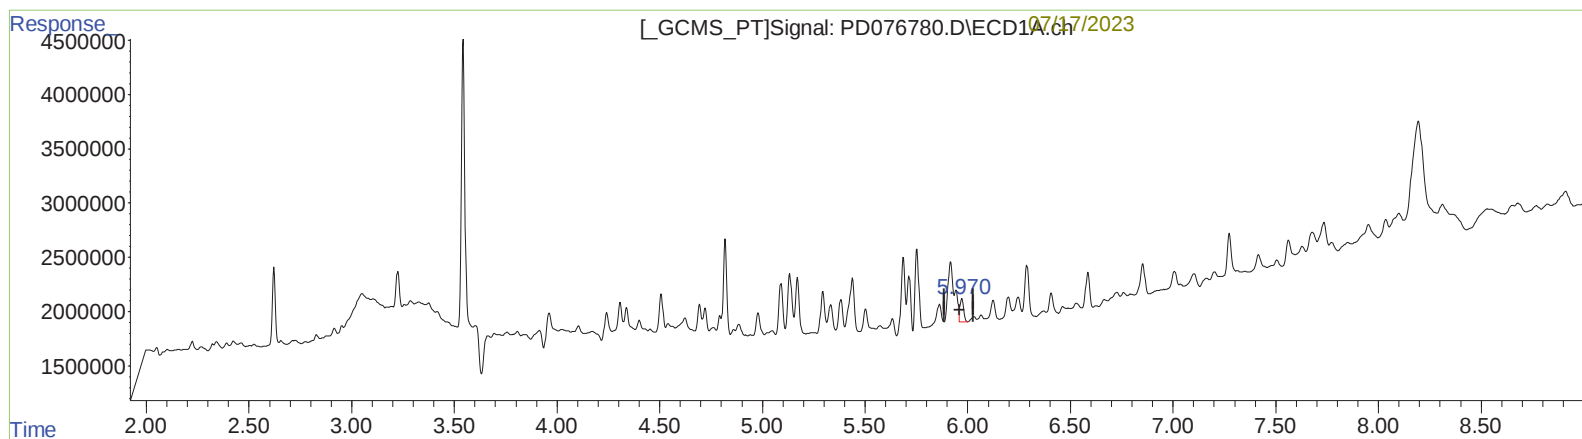

(10) trans-Chlordane (B)
 5.970min 0.891 ng/ml m
 response 2739132

(10) trans-Chlordane #2 (B)
 4.944min 1.074 ng/ml m
 response 1452236

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 16:21
Operator : AR\AJ
Sample : 03458-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
A46M2



Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 00:01:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

07/17/2023
Supervised By :Ankita
Jodhani

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

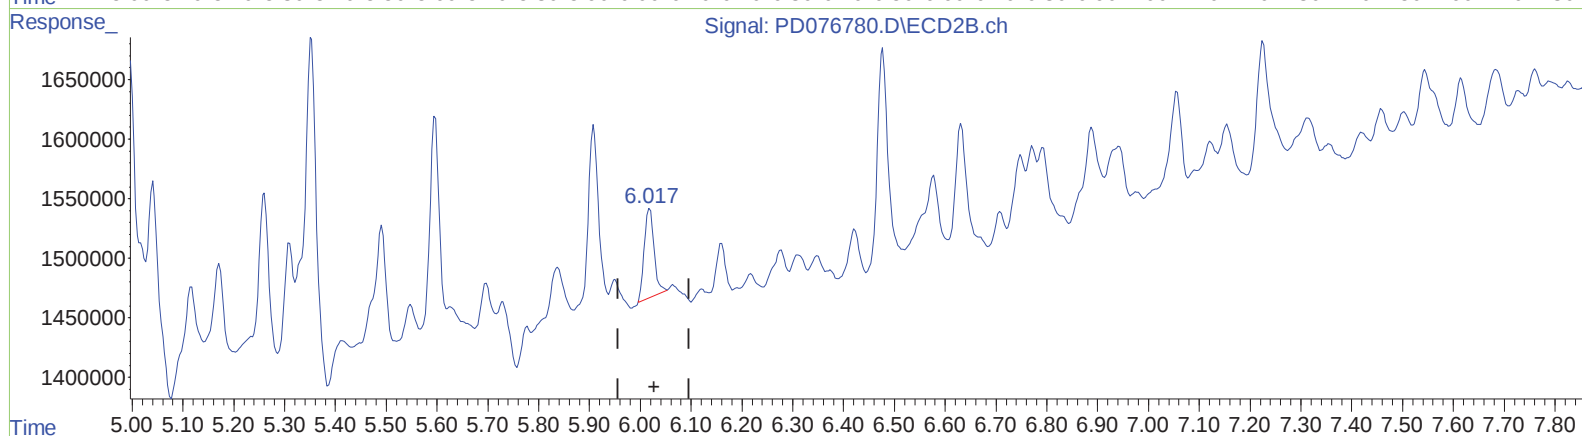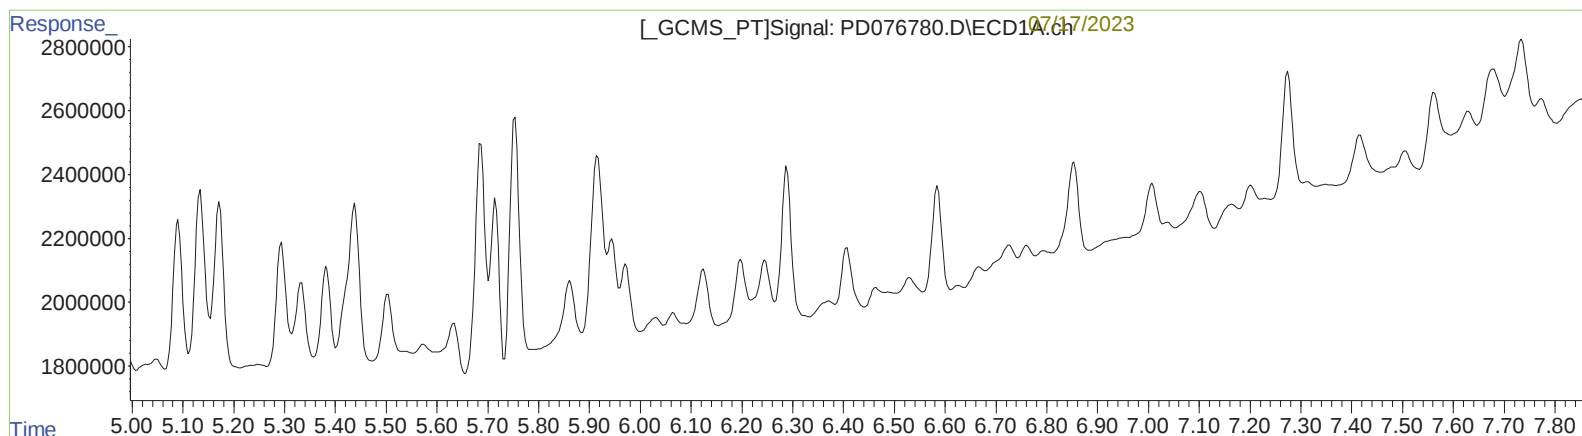

QEdit

(17) 4,4'-DDT (MA)
0.000min 0.000 ng/ml
response 0

(17) 4,4'-DDT #2 (MA)
6.019min 1.078 ng/ml
response 1010099

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 16:21
Operator : AR\AJ
Sample : 03458-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
A46M2



Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 00:01:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

07/17/2023
Supervised By :Ankita
Jodhani

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

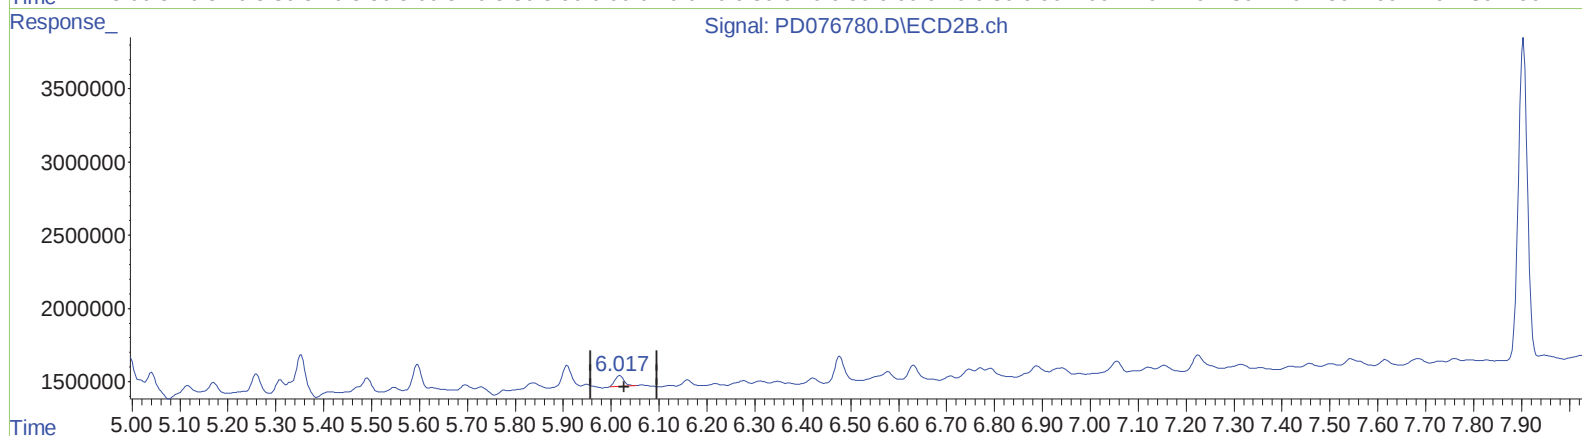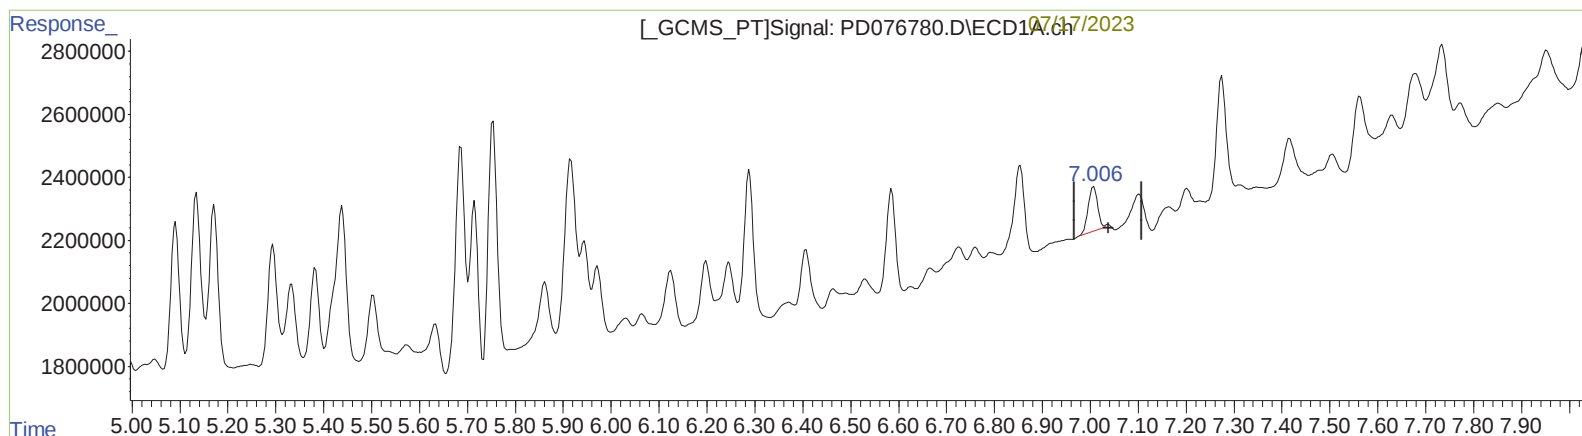

QEdit

(17) 4,4'-DDT (MA)
7.006min 0.864 ng/ml m
response 1929165

(17) 4,4'-DDT #2 (MA)
6.019min 1.078 ng/ml
response 1010099