

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
 Data File : PD076794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 19:42
 Operator : AR\AJ
 Sample : 03458-22MS
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46K5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 00:06:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	2.764	329.2E6	13715733	154.764m	12.849 #
27)	SA Decachlor...	9.082	7.903	64906993	27050496	26.716	25.234
Target Compounds							
2)	A alpha-BHC	3.999	3.265	189.1E6	80419612	53.340m	50.823
3)	MA gamma-BHC...	4.334	3.593	250.6E6	82617000	75.560m	55.147m#
4)	MA Heptachlor	4.923	3.934	173.7E6	139.7E6	49.965m	93.464 #
5)	MB Aldrin	5.268	4.214	174.2E6	81575891	50.945	54.204m
6)	B beta-BHC	4.520	3.892	73814285	27578457	48.563m	38.497
7)	B delta-BHC	4.779	4.122	173.4E6	88264220	51.715m	57.829
8)	B Heptachlo...	5.694	4.716	175.6E6	78897282	58.622	56.080
9)	A Endosulfan I	6.082	5.087	145.3E6	56426144	51.010	45.542
10)	B trans-Chl...	5.951	4.965	164.1E6	67755601	53.373m	50.106m
11)	B cis-Chlor...	6.031	5.031	159.8E6	63589687	50.404	45.073
12)	B 4,4'-DDE	6.203	5.220	311.8E6	127.3E6	107.037	105.321
13)	MA Dieldrin	6.357	5.351	336.4E6	162.0E6	106.619	116.187
14)	MA Endrin	6.588	5.627	279.8E6	120.7E6	108.555	97.586
15)	B Endosulfa...	6.808	5.921	268.3E6	119.4E6	100.903	99.318
16)	A 4,4'-DDD	6.722	5.774	267.5E6	107.3E6	118.404	113.218
17)	MA 4,4'-DDT	7.035	6.025	243.0E6	108.2E6	108.822m	115.520
18)	B Endrin al...	6.938	6.101	179.9E6	73711834	96.195	87.877
19)	B Endosulfa...	7.173	6.323	252.4E6	111.5E6	101.059	99.928
20)	A Methoxychlor	7.512	6.600	656.5E6	263.7E6	495.948	494.225
21)	B Endrin ke...	7.660	6.830	266.8E6	129.3E6	96.353	101.052

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 19:42
Operator : AR\AJ
Sample : 03458-22MS
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 00:06:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

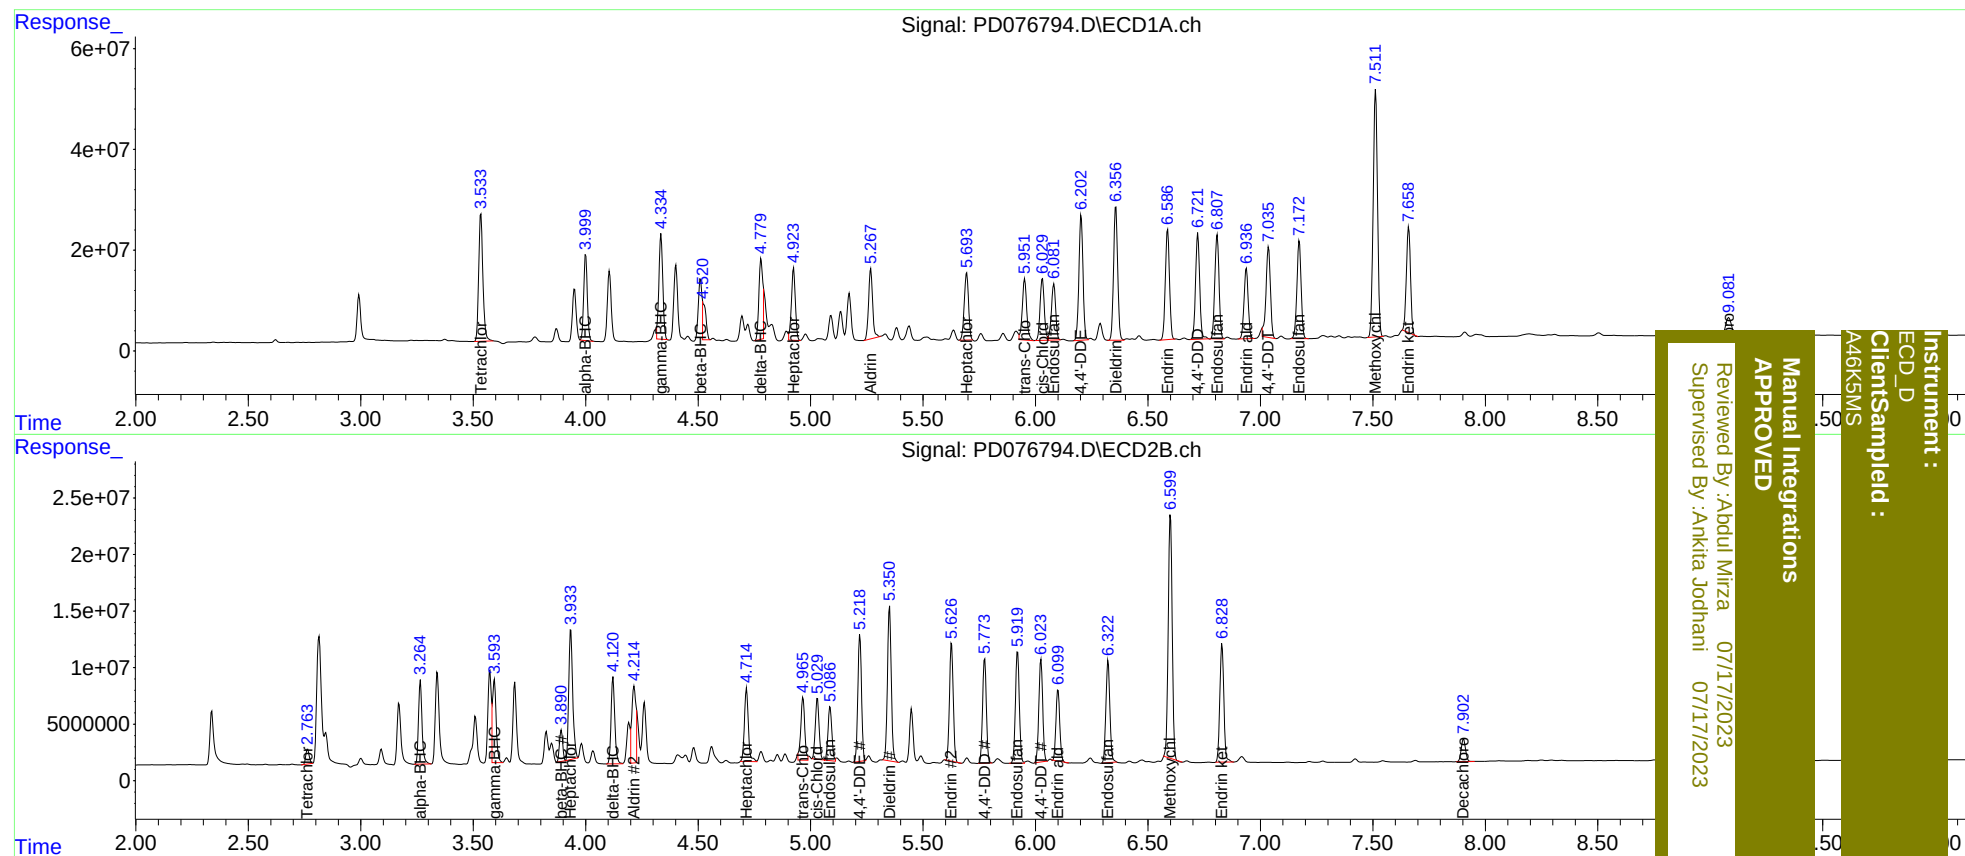

Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
A46K5MS