

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
 Data File : PD076795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 19:56
 Operator : AR\AJ
 Sample : 03458-23MSD
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46K5MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 00:07:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.765	322.2E6	13450722	151.469m	12.601 #
27)	SA Decachlor...	9.084	7.904	62499149	25853436	25.725	24.118
Target Compounds							
2)	A alpha-BHC	3.999	3.266	193.2E6	82142029	54.500m	51.911
3)	MA gamma-BHC...	4.334	3.593	260.8E6	81107745	78.638m	54.139m#
4)	MA Heptachlor	4.923	3.934	171.3E6	139.2E6	49.286m	93.094 #
5)	MB Aldrin	5.268	4.214	175.8E6	91069514	51.404	60.512m
6)	B beta-BHC	4.522	3.892	65958548	28191181	43.395m	39.352
7)	B delta-BHC	4.779	4.122	175.7E6	88689030	52.389m	58.107
8)	B Heptachlo...	5.694	4.716	175.8E6	78774635	58.681	55.993
9)	A Endosulfan I	6.082	5.087	144.6E6	56900788	50.772	45.925
10)	B trans-Chl...	5.950	4.965	161.6E6	69828927	52.548m	51.640m
11)	B cis-Chlor...	6.031	5.031	158.8E6	63752197	50.100	45.188
12)	B 4,4'-DDE	6.203	5.219	309.4E6	128.2E6	106.214	106.053
13)	MA Dieldrin	6.357	5.351	334.2E6	161.7E6	105.904	115.921
14)	MA Endrin	6.588	5.627	279.1E6	120.3E6	108.274	97.319
15)	B Endosulfa...	6.808	5.921	268.4E6	119.6E6	100.960	99.463
16)	A 4,4'-DDD	6.722	5.774	268.5E6	108.0E6	118.816	113.978
17)	MA 4,4'-DDT	7.036	6.025	240.0E6	107.7E6	107.489m	114.937
18)	B Endrin al...	6.938	6.100	181.1E6	74744984	96.838	89.109
19)	B Endosulfa...	7.173	6.323	251.4E6	111.5E6	100.660	99.928
20)	A Methoxychlor	7.513	6.601	654.1E6	262.0E6	494.107	490.984
21)	B Endrin ke...	7.659	6.830	267.4E6	129.5E6	96.562	101.202

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071523\
Data File : PD076795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 19:56
Operator : AR\AJ
Sample : 03458-23MSD
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 00:07:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

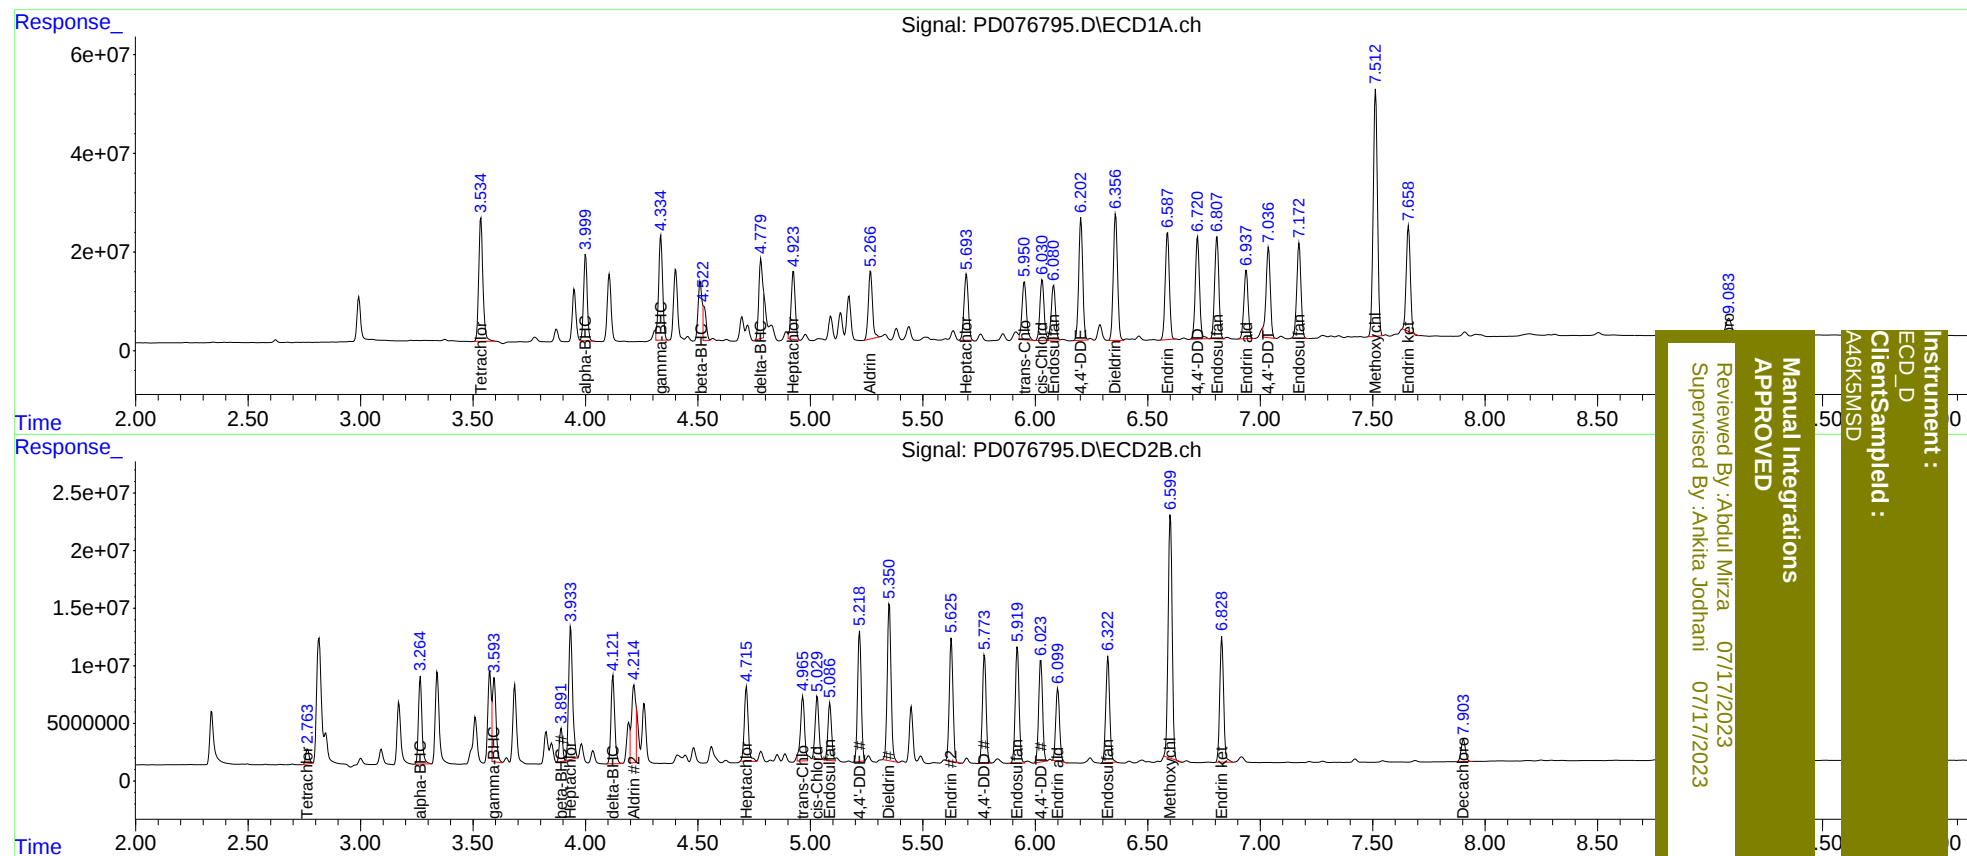

Instrument :
ECD_D
Client Sampled :
A46K5MSD

Manual Integrations
APPROVED

Reviewed By : Abdul Miza 07/17/2023
Supervised By : Ankita Jodhani 07/17/2023