

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
 Data File : PD083927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 10:43
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:24:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 04:22:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.771	0	12459	N.D.	0.002 #
28)	SA Decachlor...	0.000	7.898	0	162569	N.D.	0.025 #
Target Compounds							
5)	MB Aldrin	5.319f	0.000	73495	0	0.036	N.D. #
7)	B delta-BHC	4.827f	0.000	573334	0	0.315	N.D. #
9)	A Endosulfan I	0.000	5.105f	0	462536	N.D.	0.067 #
14)	MA Endrin	0.000	5.647f	0	670829	N.D.	0.101 #
18)	B Endrin al...	0.000	6.103	0	757248	N.D.	0.151 #
20)	A Methoxychlor	0.000	6.572f	0	229330	N.D.	0.078 #
21)	B Endrin ke...	7.656f	0.000	132977	0	0.064	N.D. #
22)	Mirex	8.173f	7.009	436061	309958	0.268	0.057 #
24)	Chlordane-2	0.000	4.302f	0	1789978	N.D.	6.378 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
Data File : PD083927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 10:43
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:24:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 04:22:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

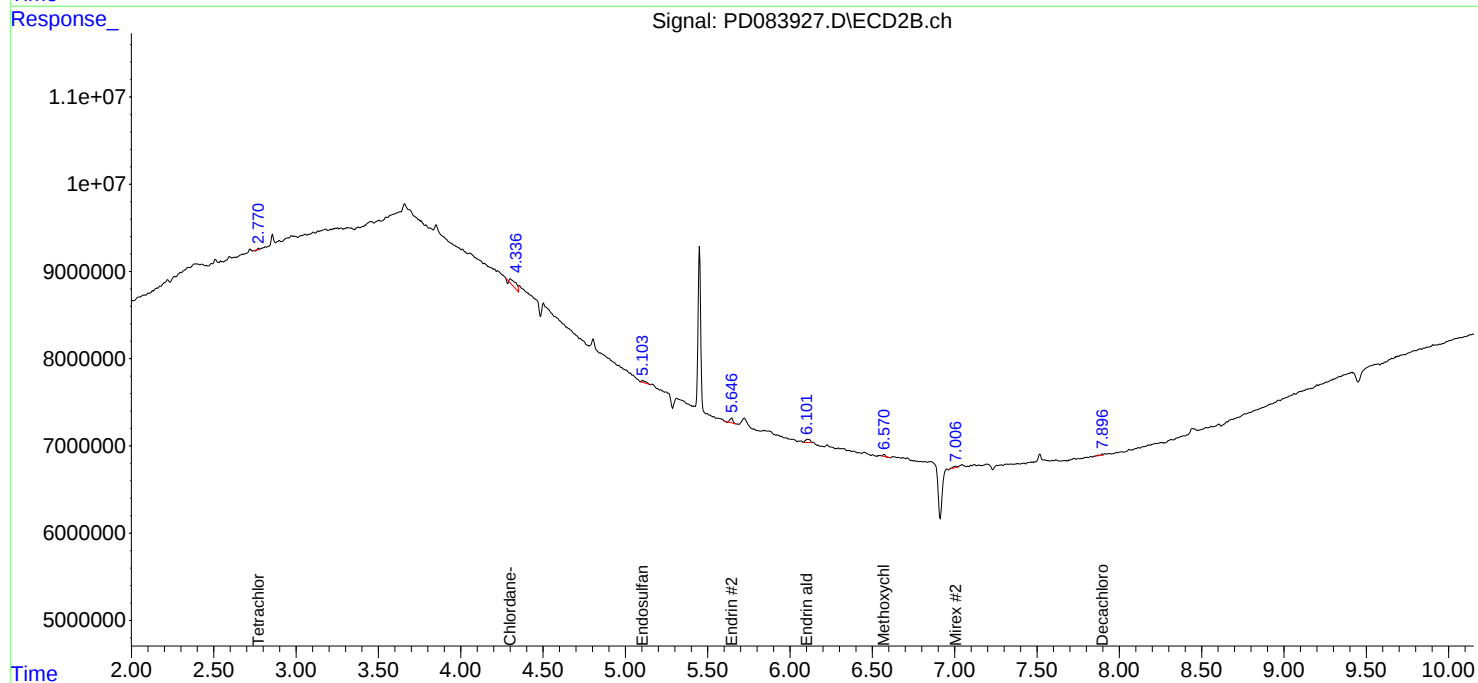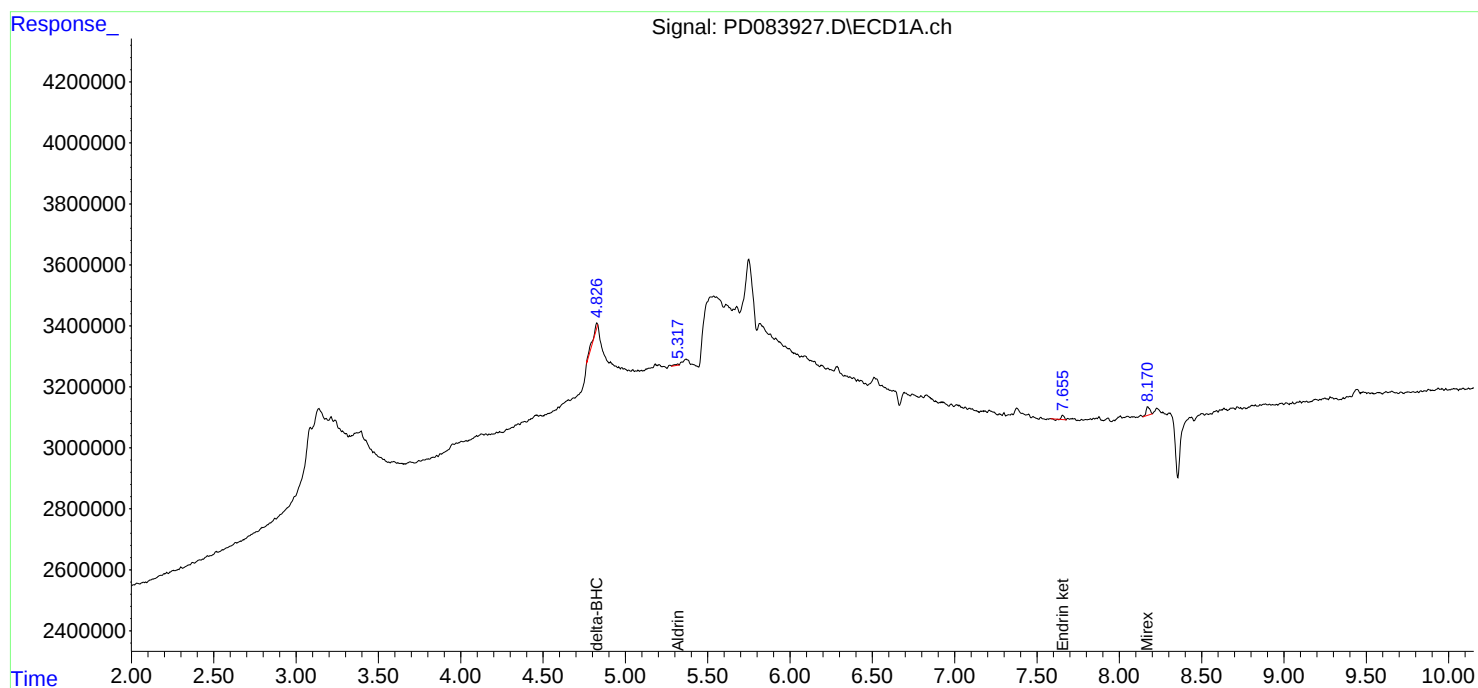


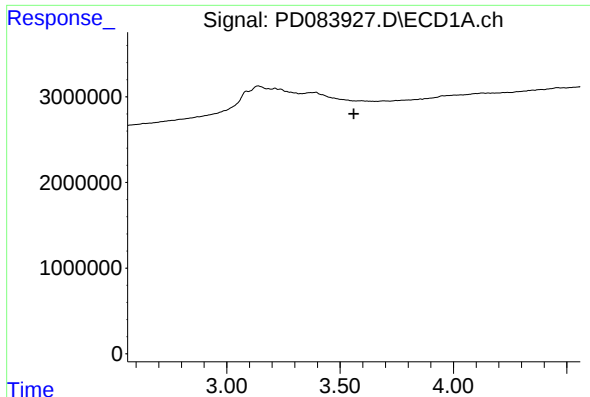

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.561 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

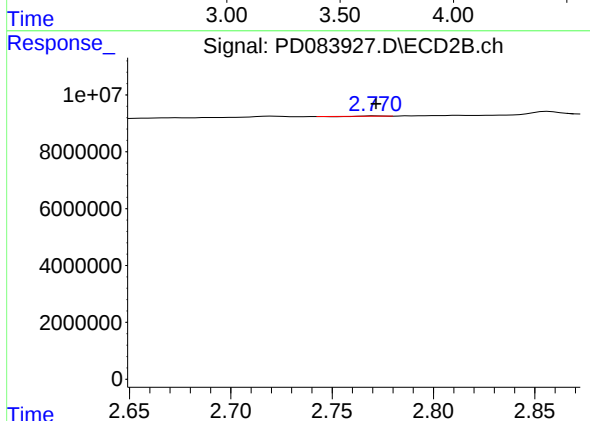


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 12459
Conc: 0.00 ng/ml

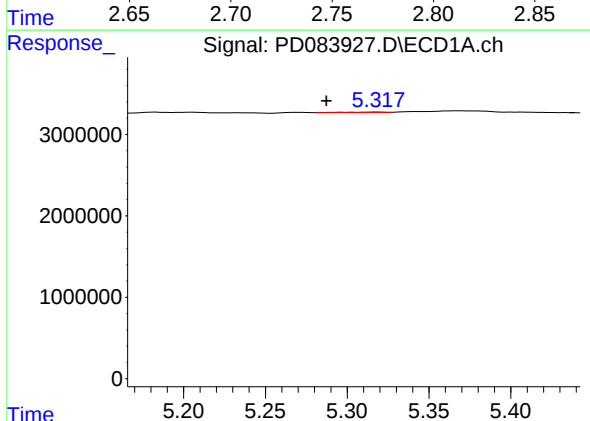


#5 Aldrin

R.T.: 5.319 min
Delta R.T.: 0.031 min
Response: 73495
Conc: 0.04 ng/ml

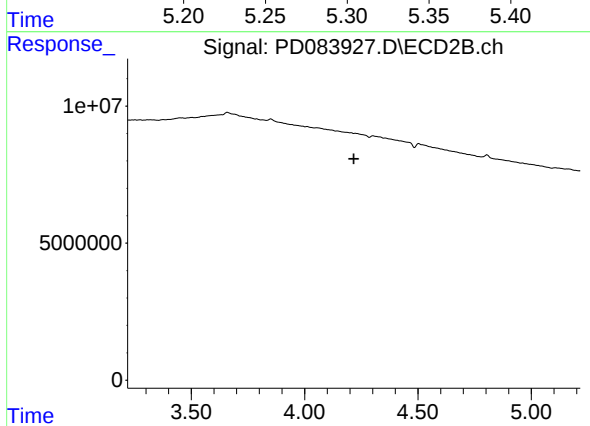

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.217 min
Response: 0
Conc: N.D.

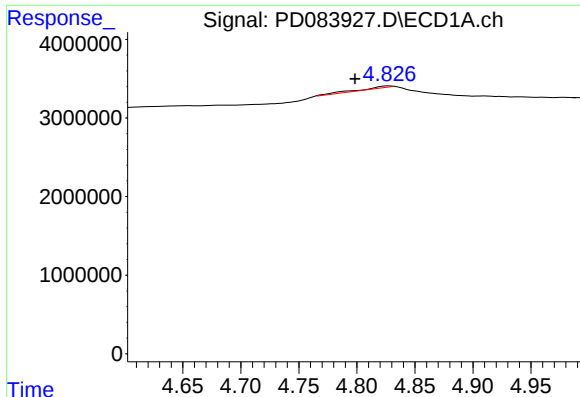

#7 delta-BHC


R.T.: 4.827 min
Delta R.T.: 0.029 min
Response: 573334
Conc: 0.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

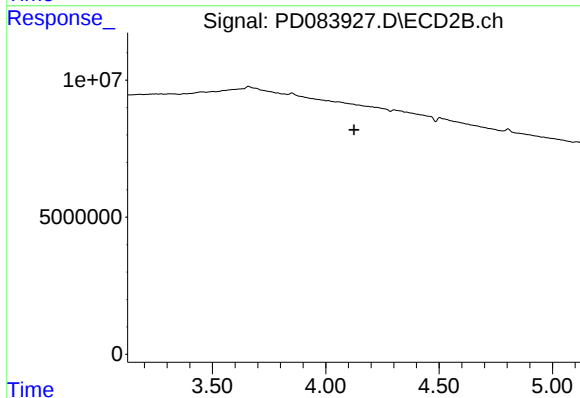


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.126 min
Response: 0
Conc: N.D.

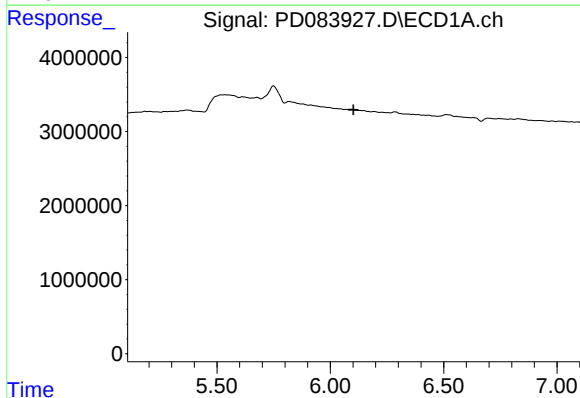


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.103 min
Response: 0
Conc: N.D.

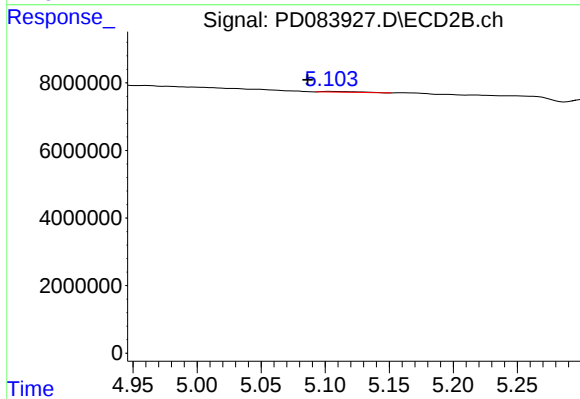

#9 Endosulfan I


R.T.: 5.105 min
Delta R.T.: 0.018 min
Response: 462536
Conc: 0.07 ng/ml

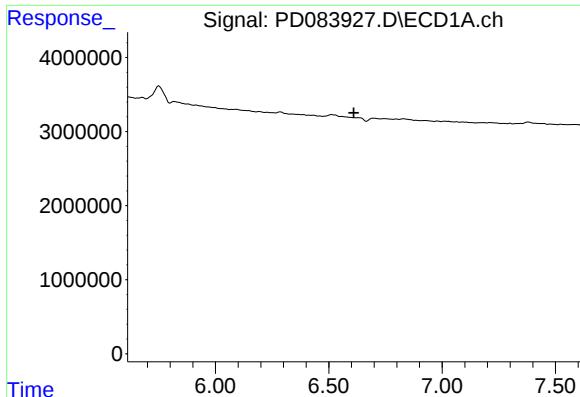

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

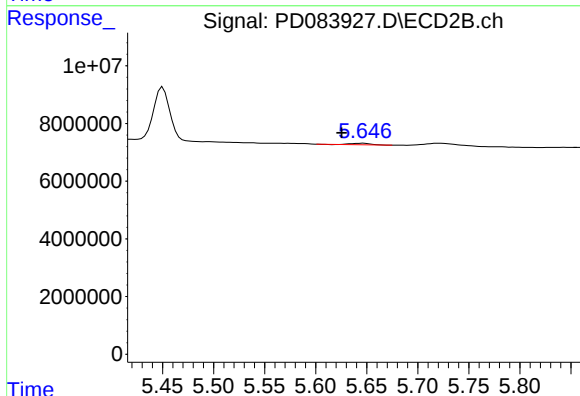


#14 Endrin

R.T.: 5.647 min
Delta R.T.: 0.021 min
Response: 670829
Conc: 0.10 ng/ml

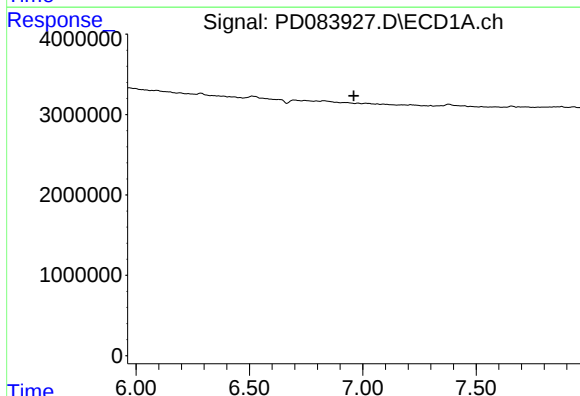


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.960 min
Response: 0
Conc: N.D.

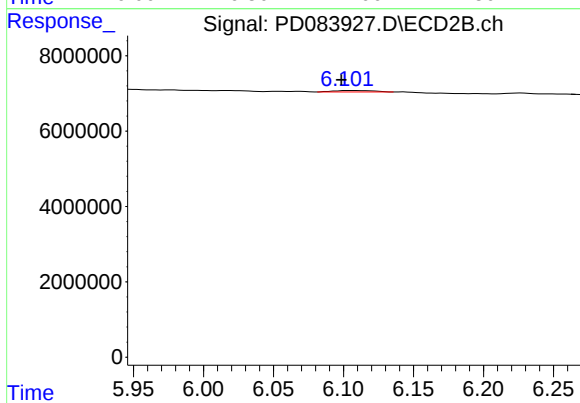

#18 Endrin aldehyde


R.T.: 6.103 min
Delta R.T.: 0.004 min
Response: 757248
Conc: 0.15 ng/ml

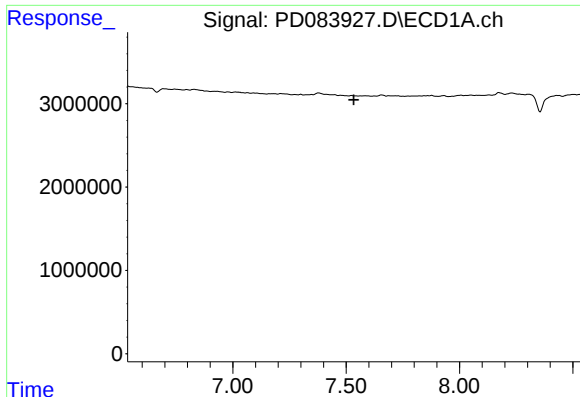

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

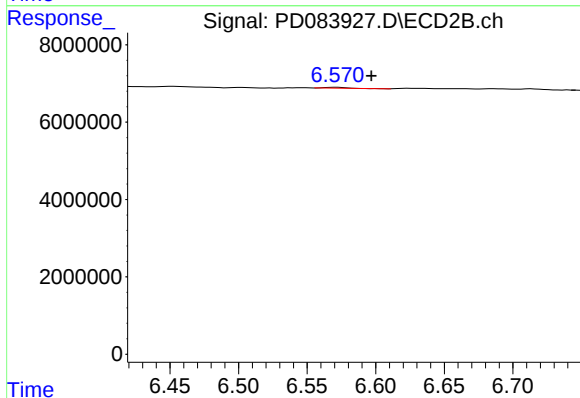


#20 Methoxychlor

R.T.: 6.572 min
Delta R.T.: -0.025 min
Response: 229330
Conc: 0.08 ng/ml

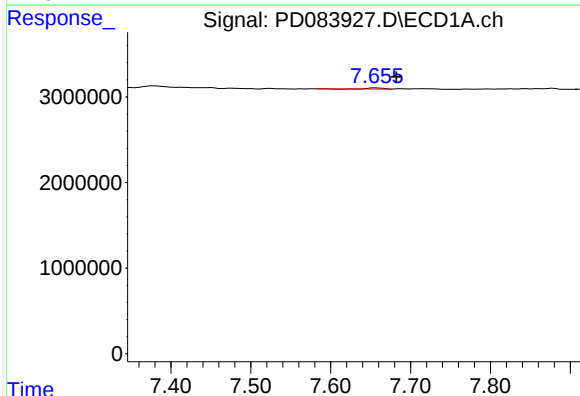


#21 Endrin ketone

R.T.: 7.656 min
Delta R.T.: -0.026 min
Response: 132977
Conc: 0.06 ng/ml

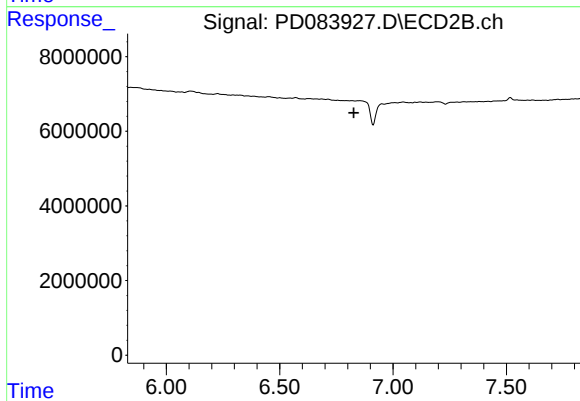

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.827 min
Response: 0
Conc: N.D.

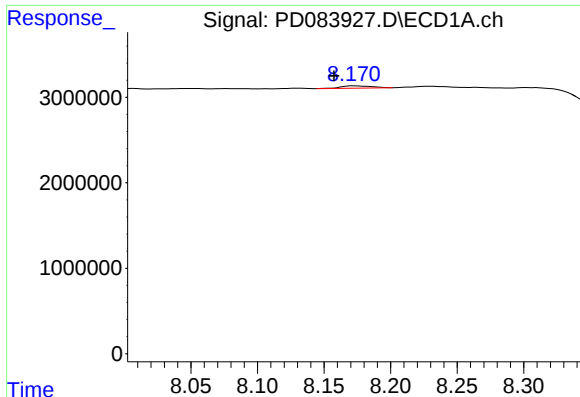

#22 Mirex


R.T.: 8.173 min
Delta R.T.: 0.016 min
Response: 436061
Conc: 0.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

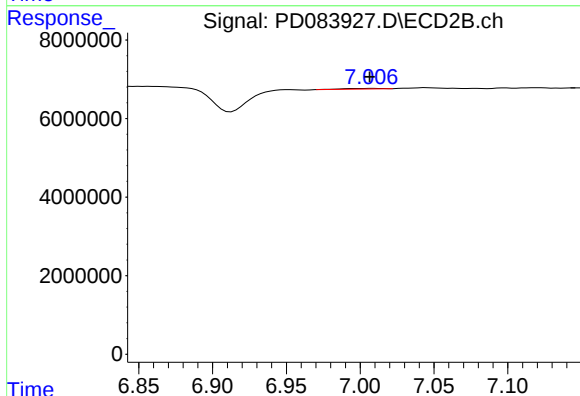


#22 Mirex

R.T.: 7.009 min
Delta R.T.: 0.002 min
Response: 309958
Conc: 0.06 ng/ml

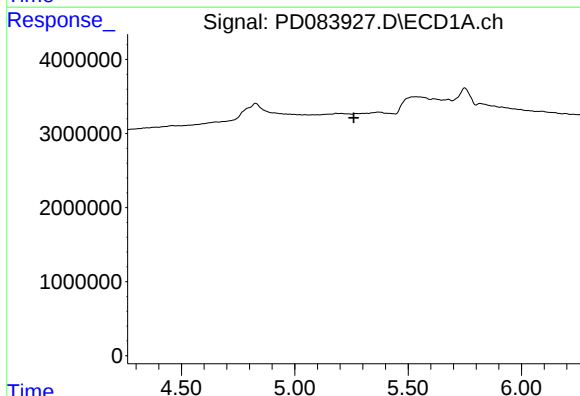


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.260 min
Response: 0
Conc: N.D.

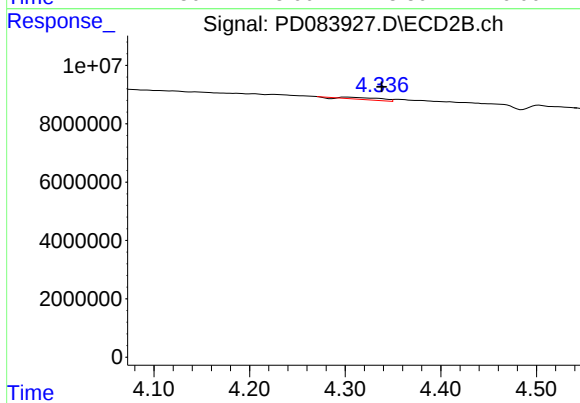

#24 Chlordane-2


R.T.: 4.302 min
Delta R.T.: -0.037 min
Response: 1789978
Conc: 6.38 ng/ml

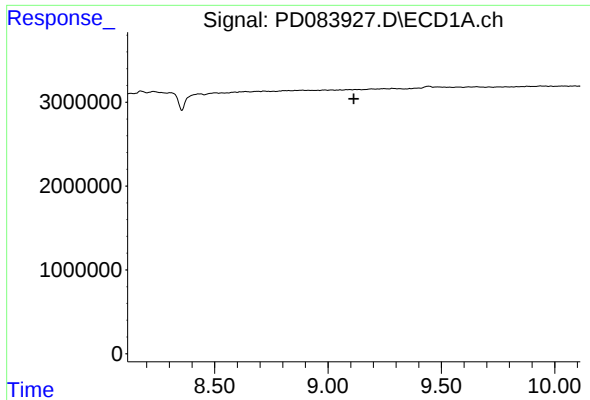

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

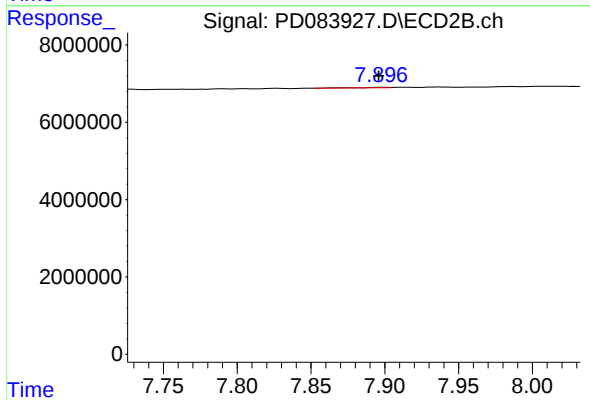

#28 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: 0.002 min
Response: 162569
Conc: 0.03 ng/ml