

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
 Data File : PD083937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 12:55
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:02:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 02:00:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	75400109	492.1E6	75.177	74.999
28)	SA Decachlor...	9.114	7.896	160.3E6	448.1E6	74.066	72.848
Target Compounds							
23)	Chlordane-1	4.728	3.764	46994014	172.6E6	763.802	749.182
24)	Chlordane-2	5.261	4.338	50546103	197.3E6	744.390	737.229
25)	Chlordane-3	5.973	4.966	226.3E6	570.9E6	769.080	747.561
26)	Chlordane-4	6.055	5.029	273.8E6	557.5E6	766.706	741.419
27)	Chlordane-5	6.908	5.924	50947926	204.7E6	756.399	748.701



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
Data File : PD083937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 12:55
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:02:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 02:00:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

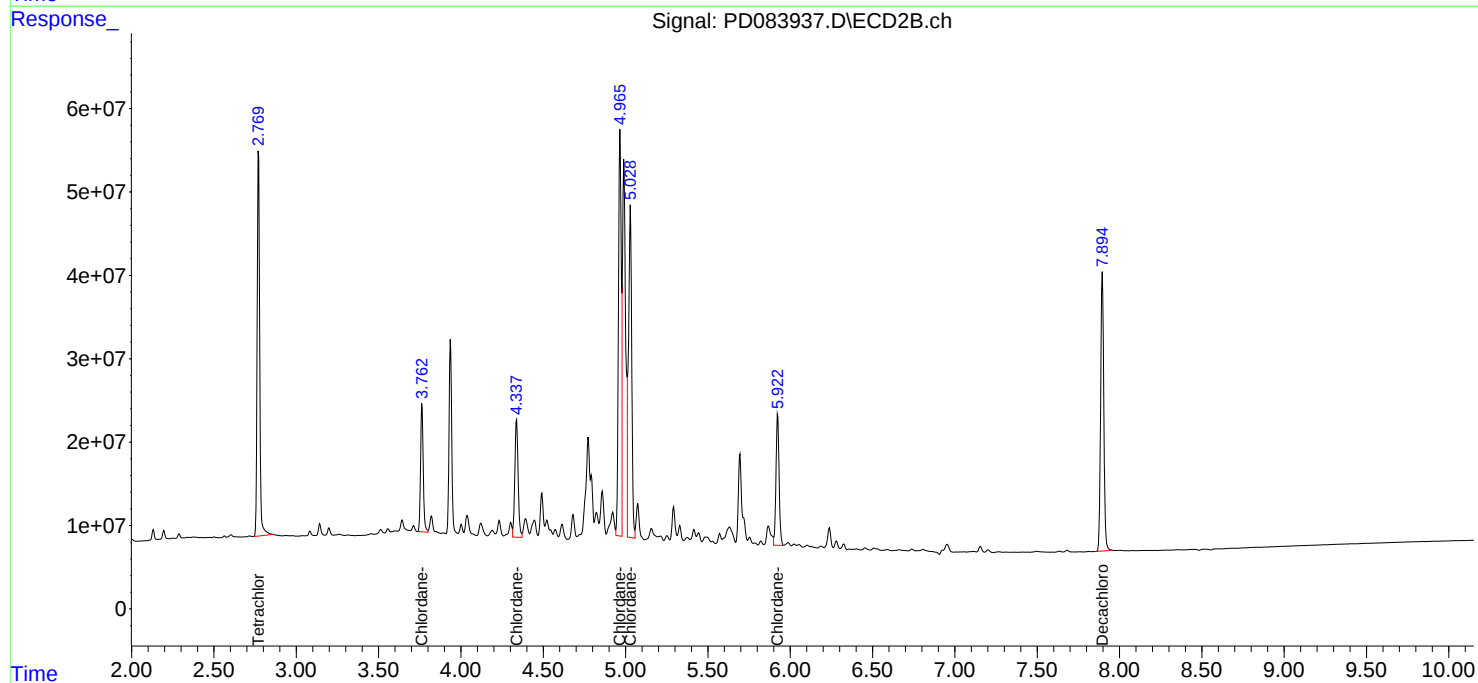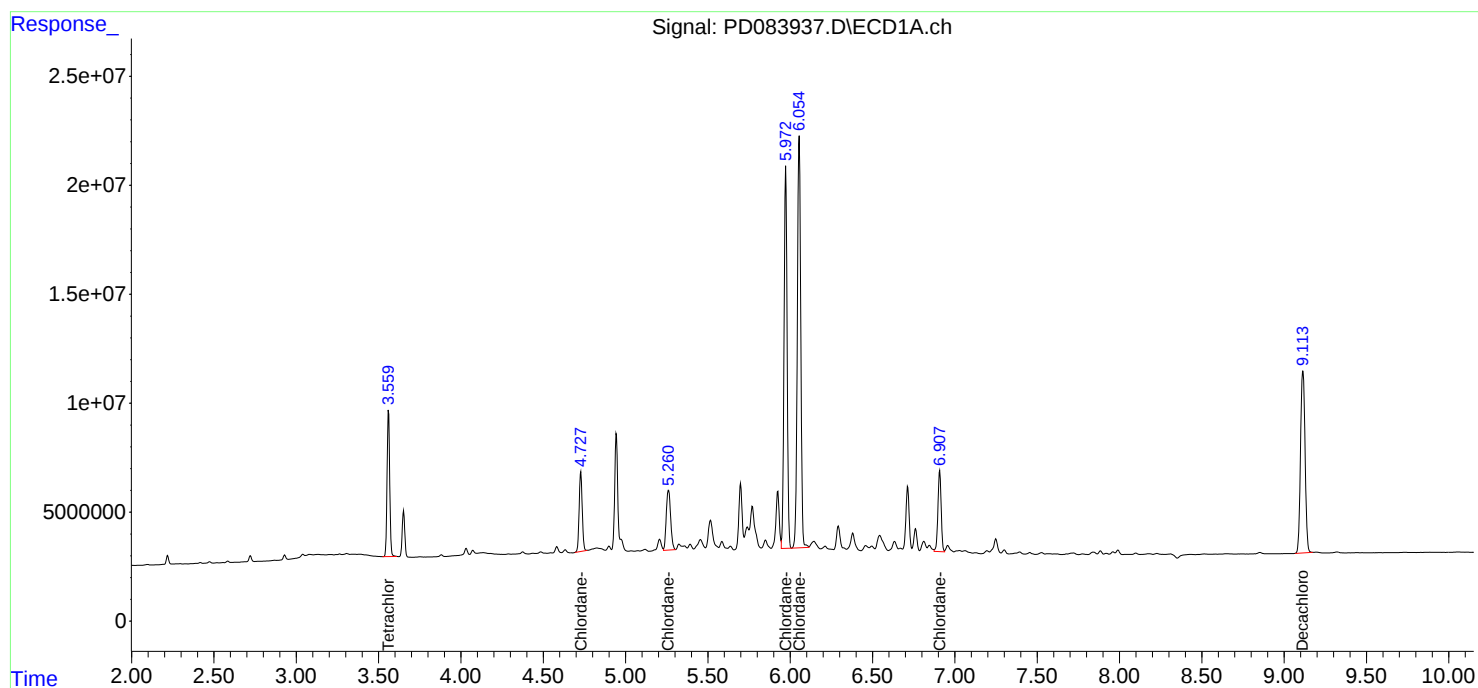


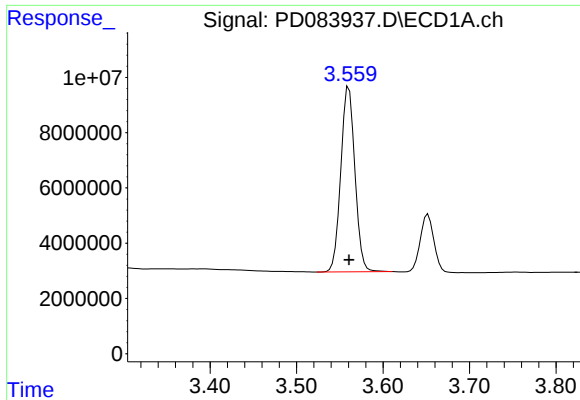

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 75400109
Conc: 75.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

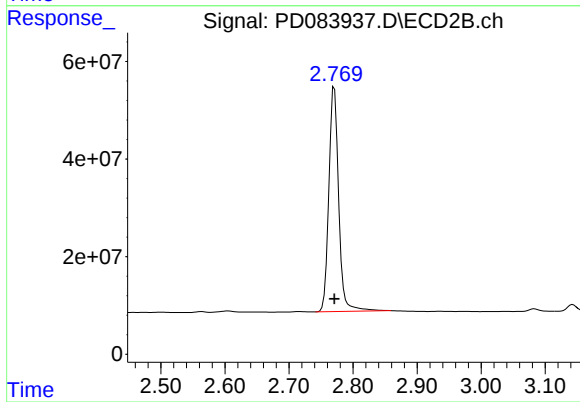


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 492134785
Conc: 75.00 ng/ml

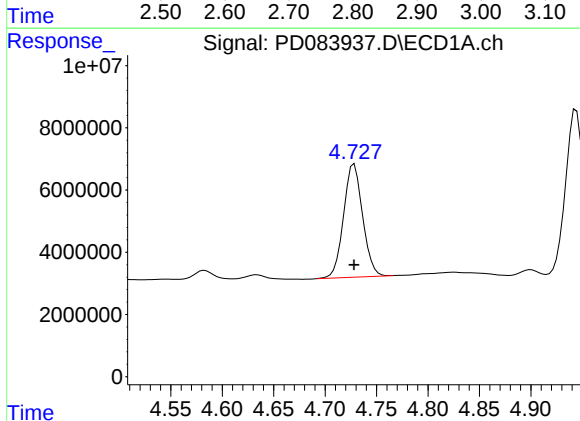


#23 Chlordane-1

R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 46994014
Conc: 763.80 ng/ml

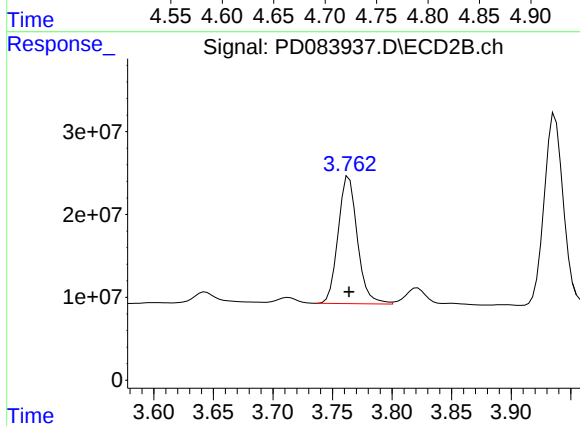

#23 Chlordane-1


R.T.: 3.764 min
Delta R.T.: 0.000 min
Response: 172624535
Conc: 749.18 ng/ml

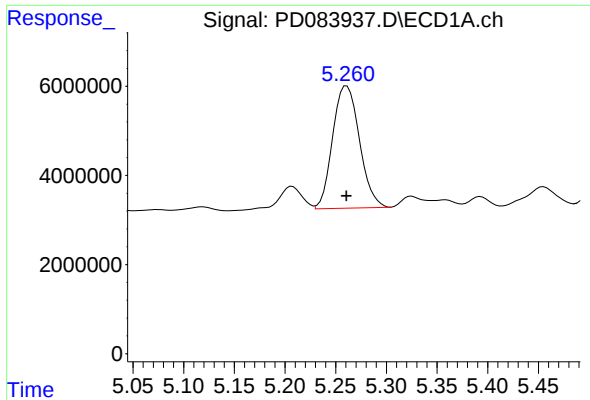

#24 Chlordane-2


R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 50546103
Conc: 744.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

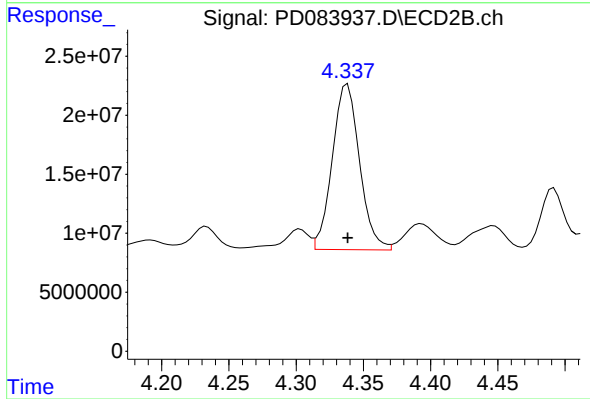


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 197284129
Conc: 737.23 ng/ml

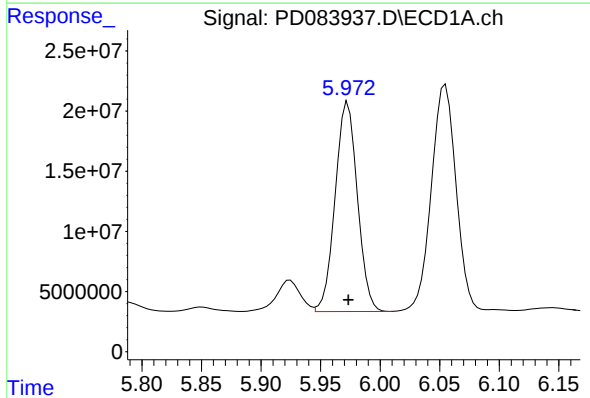


#25 Chlordane-3

R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 226314608
Conc: 769.08 ng/ml

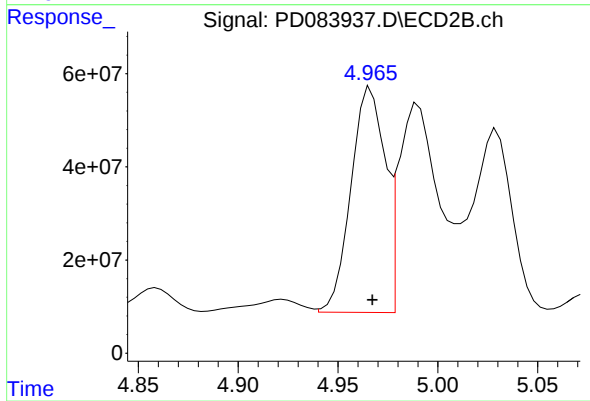

#25 Chlordane-3


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 570923144
Conc: 747.56 ng/ml

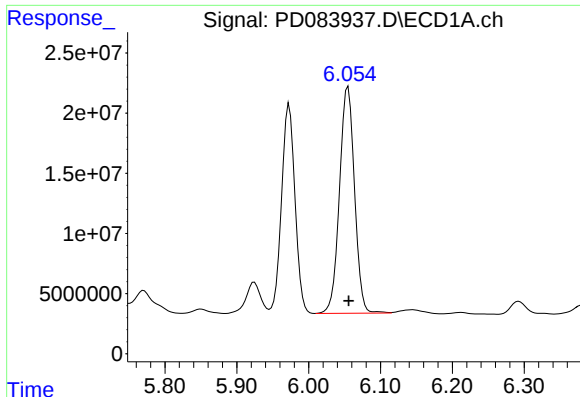

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 273798289
Conc: 766.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

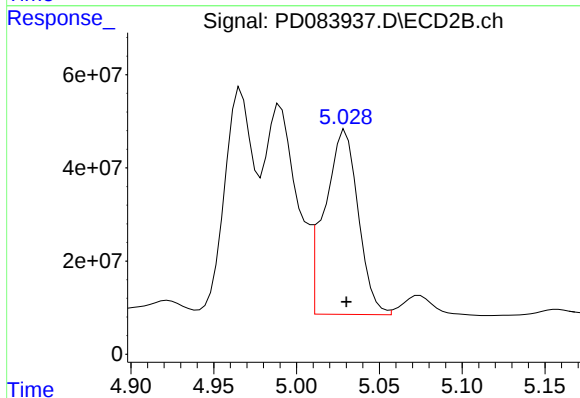


#26 Chlordane-4

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 557482927
Conc: 741.42 ng/ml

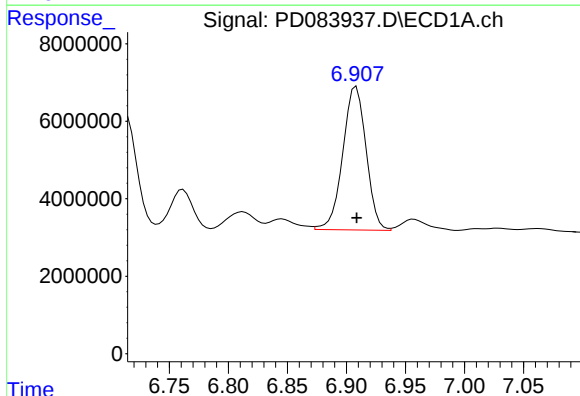


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 50947926
Conc: 756.40 ng/ml

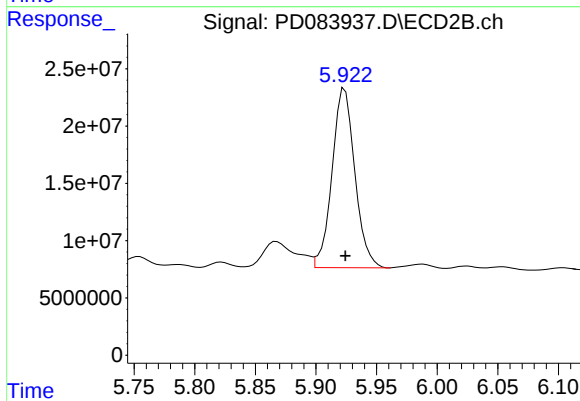

#27 Chlordane-5


R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 204732688
Conc: 748.70 ng/ml

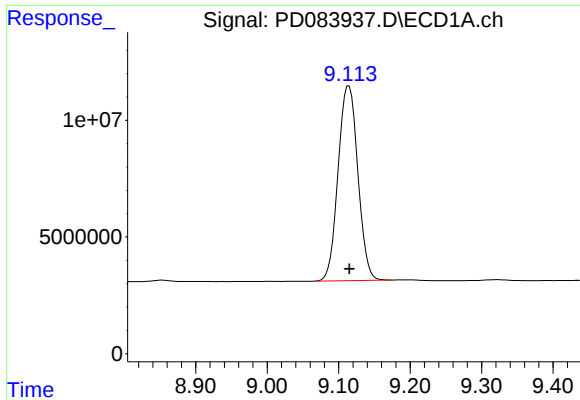

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 160319155
Conc: 74.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

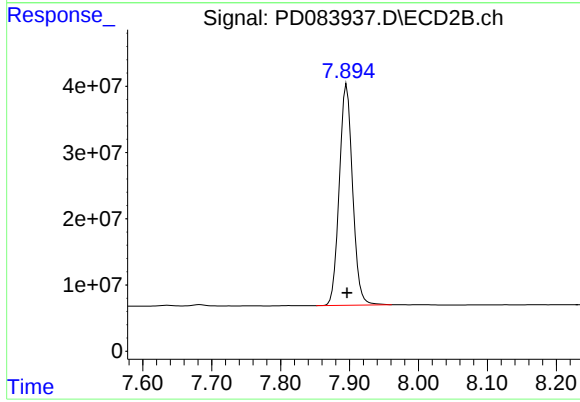

#28 Decachlorobiphenyl

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 448118225
Conc: 72.85 ng/ml