

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
 Data File : PD083938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 13:08
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:02:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 02:00:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	50148596	328.1E6	50.000	50.000
28)	SA Decachlor...	9.115	7.897	108.2E6	307.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.728	3.764	30763225	115.2E6	500.000	500.000
24)	Chlordane-2	5.260	4.338	33951344	133.8E6	500.000	500.000
25)	Chlordane-3	5.973	4.967	147.1E6	381.9E6	500.000	500.000
26)	Chlordane-4	6.056	5.030	178.6E6	376.0E6	500.000	500.000
27)	Chlordane-5	6.909	5.924	33677958	136.7E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
Data File : PD083938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 13:08
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:02:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 02:00:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

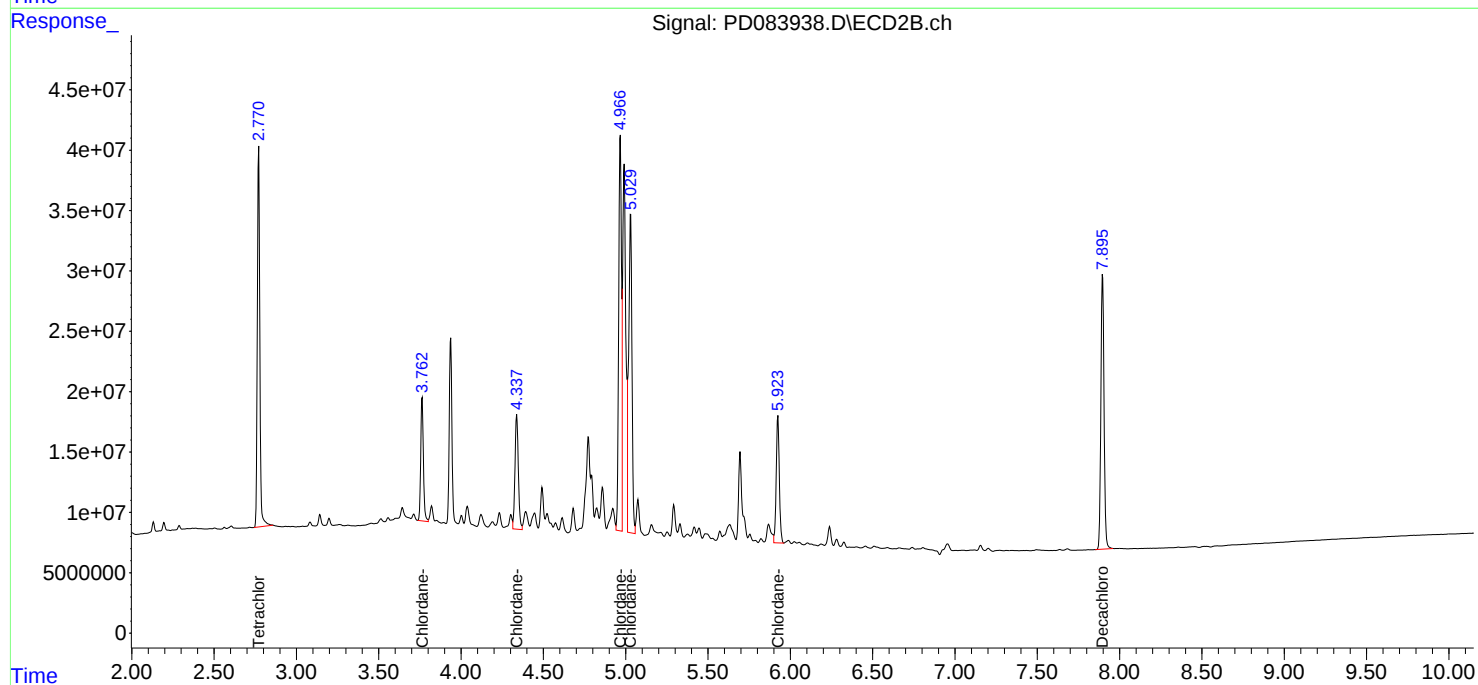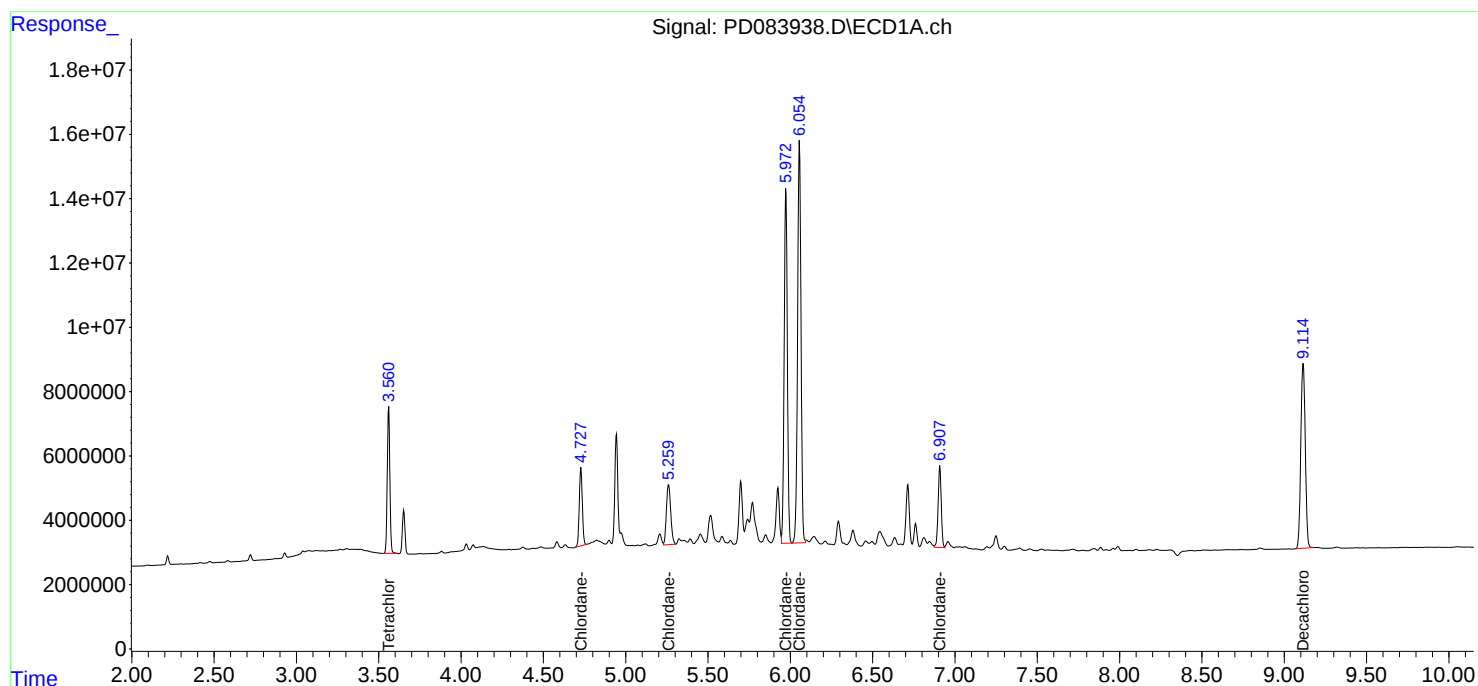


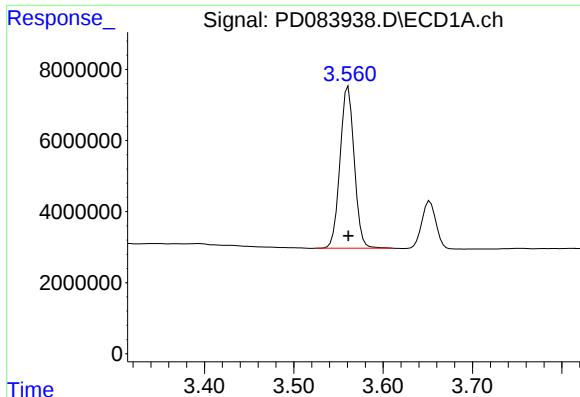

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 50148596
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

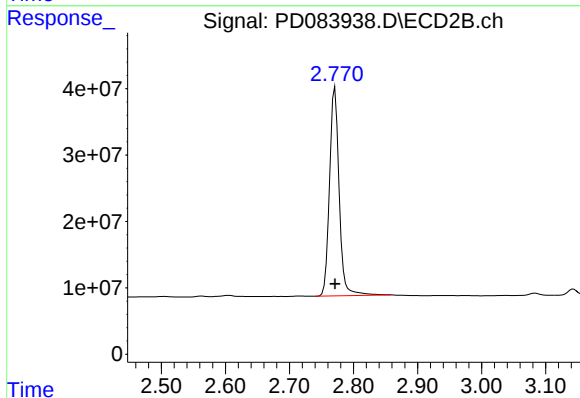


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 328092147
Conc: 50.00 ng/ml

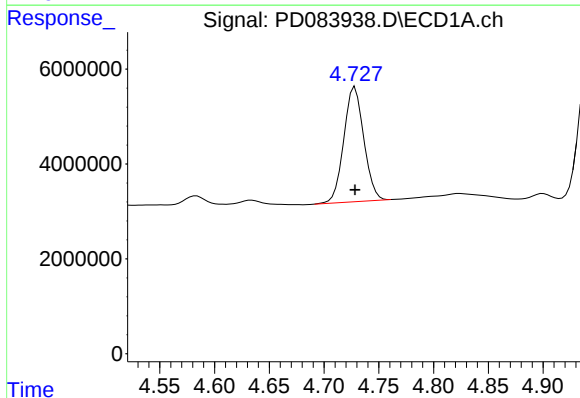


#23 Chlordane-1

R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 30763225
Conc: 500.00 ng/ml

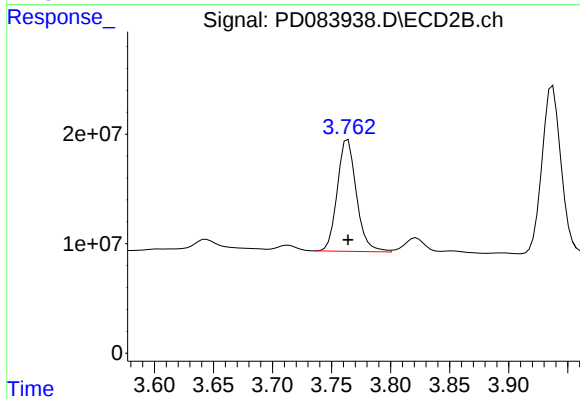

#23 Chlordane-1


R.T.: 3.764 min
Delta R.T.: 0.000 min
Response: 115208732
Conc: 500.00 ng/ml

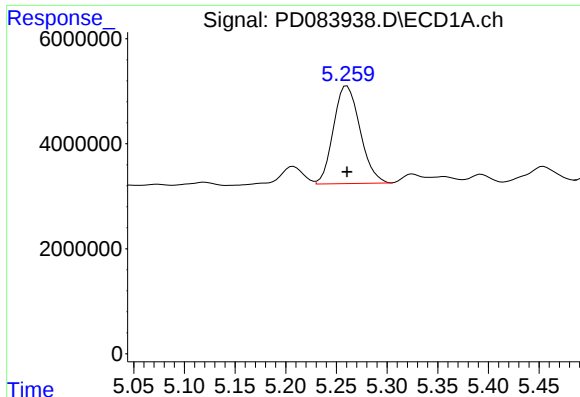

#24 Chlordane-2


R.T.: 5.260 min
Delta R.T.: 0.000 min
Response: 33951344
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

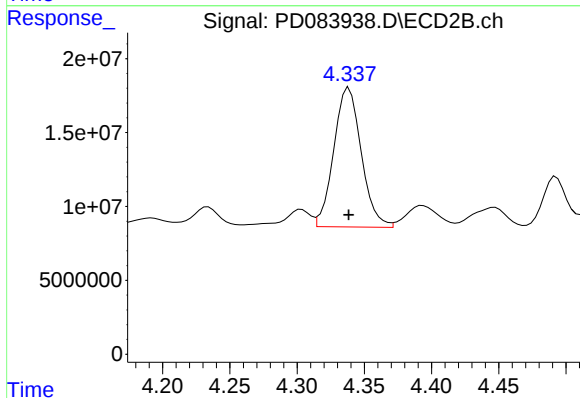


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 133801060
Conc: 500.00 ng/ml

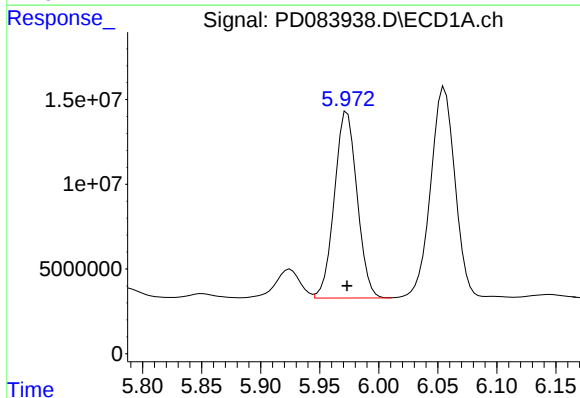


#25 Chlordane-3

R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 147133254
Conc: 500.00 ng/ml

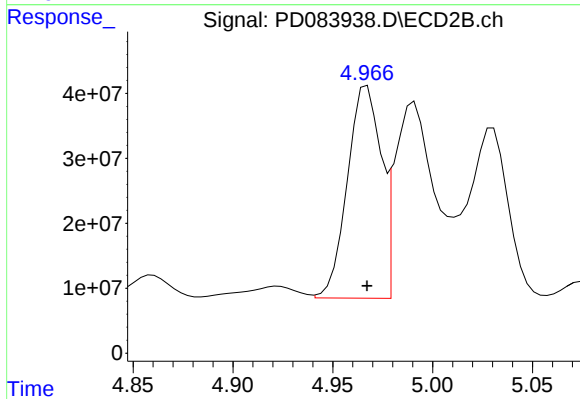

#25 Chlordane-3


R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 381857170
Conc: 500.00 ng/ml

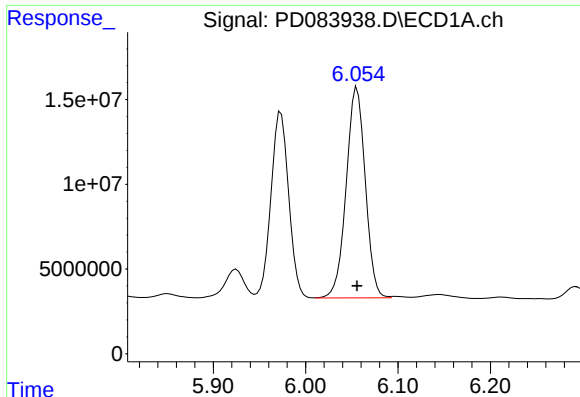

#26 Chlordane-4


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 178555044
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

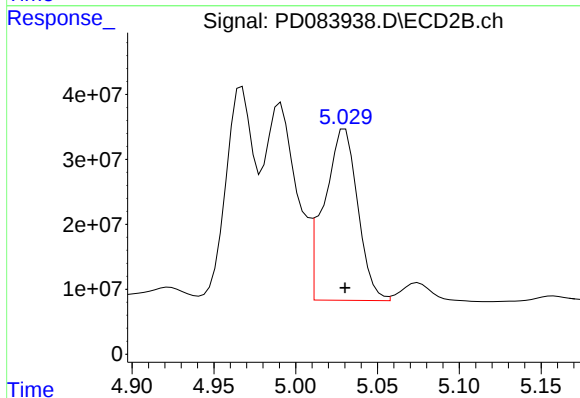


#26 Chlordane-4

R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 375956519
Conc: 500.00 ng/ml

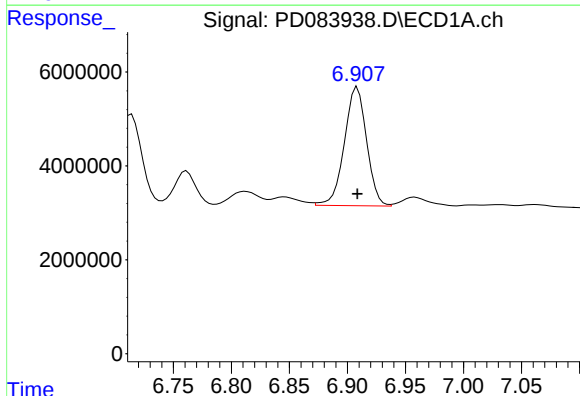


#27 Chlordane-5

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 33677958
Conc: 500.00 ng/ml

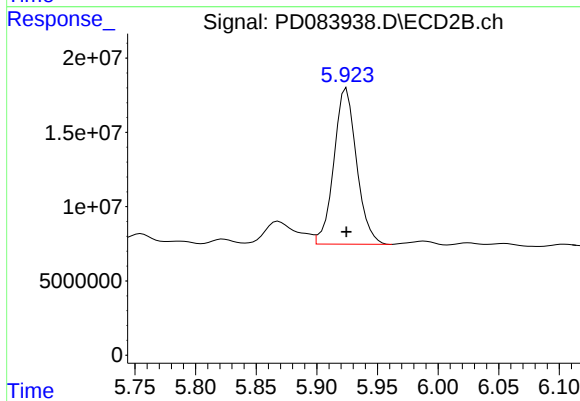

#27 Chlordane-5


R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 136725190
Conc: 500.00 ng/ml

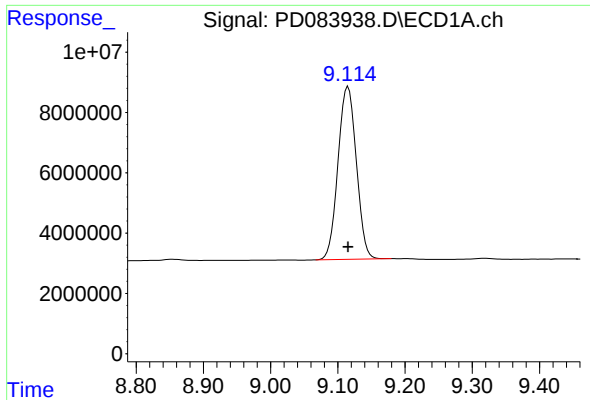

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 108227117
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

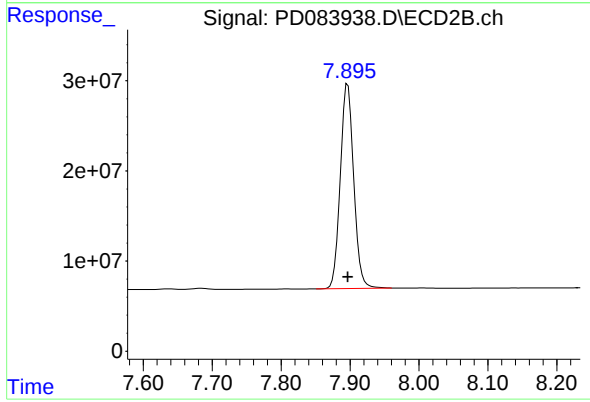

#28 Decachlorobiphenyl

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 307572747
Conc: 50.00 ng/ml