

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
 Data File : PD083947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 15:08
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD071524

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:02:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 02:00:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	52010330	341.2E6	51.856	52.002
28)	SA Decachlor...	9.115	7.897	112.5E6	319.1E6	51.979	51.873
Target Compounds							
23)	Chlordane-1	4.729	3.764	32533146	121.0E6	528.767	525.209
24)	Chlordane-2	5.261	4.339	35172609	139.6E6	517.986	521.754
25)	Chlordane-3	5.974	4.967	152.7E6	400.5E6	518.984	524.432
26)	Chlordane-4	6.056	5.031	185.5E6	394.8E6	519.366	525.034
27)	Chlordane-5	6.909	5.925	34601387	141.9E6	513.710	519.100



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071524\
Data File : PD083947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 15:08
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD071524

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:02:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 02:00:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

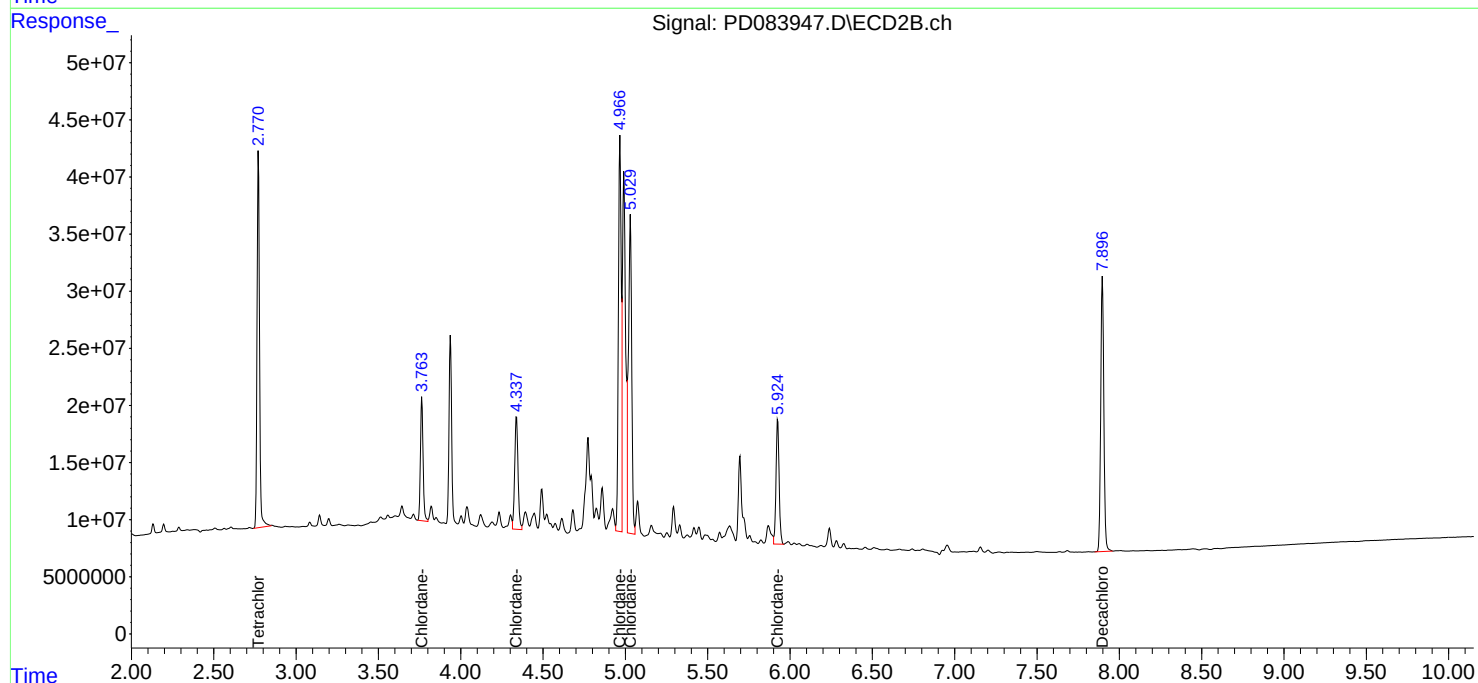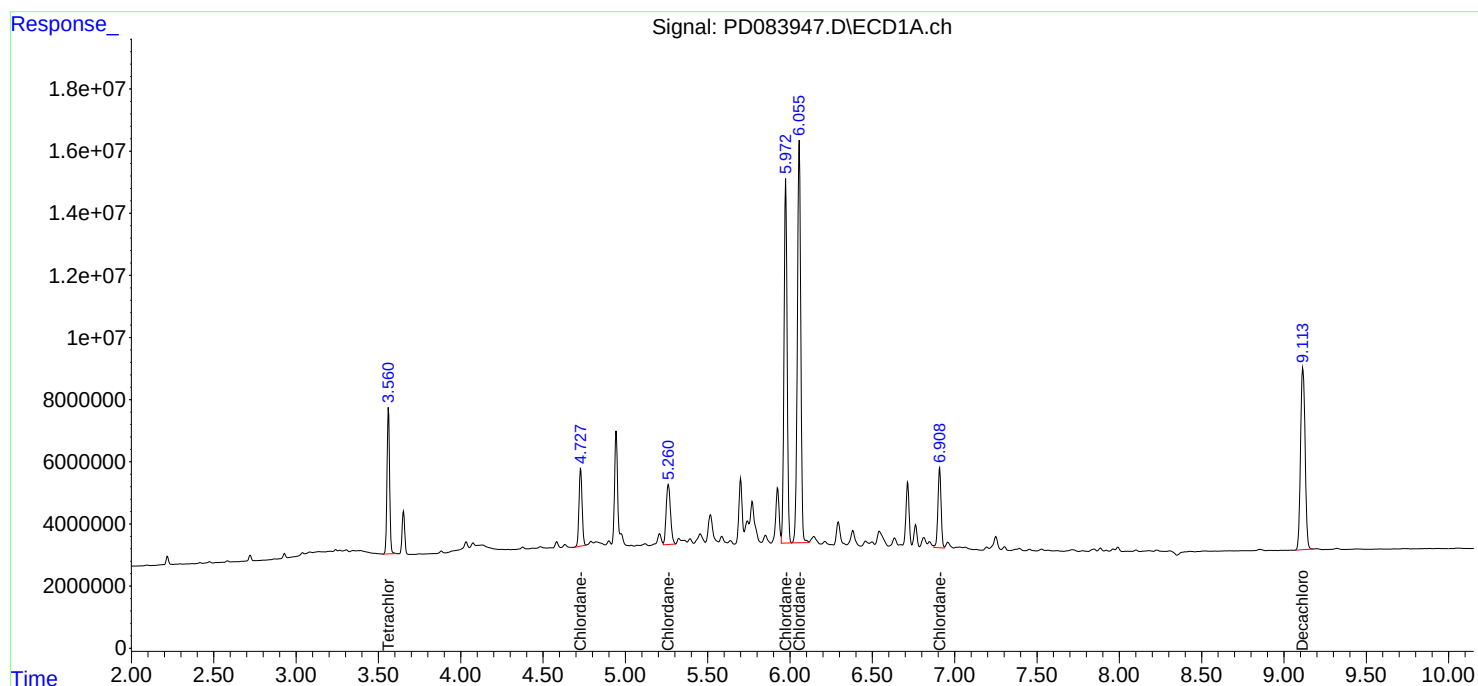


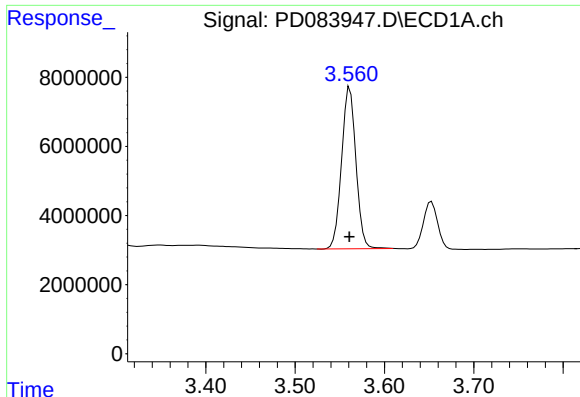

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 52010330
Conc: 51.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071524

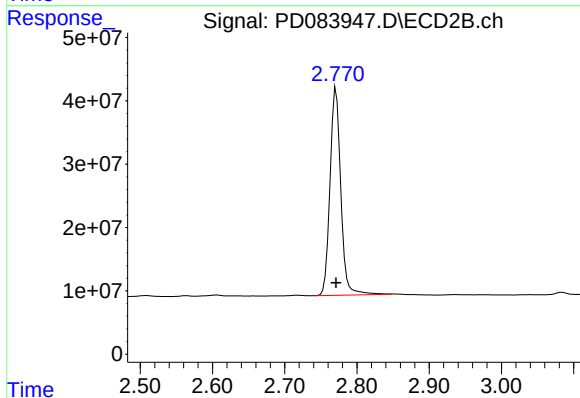


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 341228740
Conc: 52.00 ng/ml

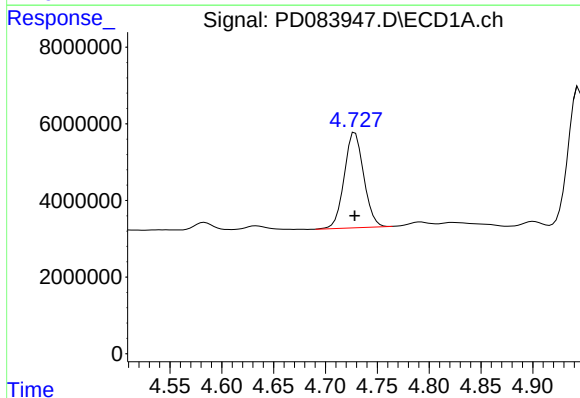


#23 Chlordane-1

R.T.: 4.729 min
Delta R.T.: 0.000 min
Response: 32533146
Conc: 528.77 ng/ml

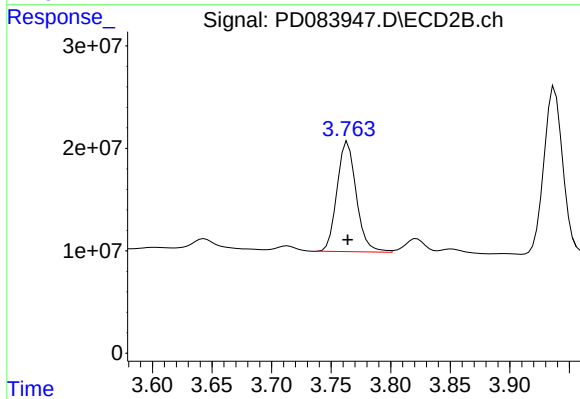

#23 Chlordane-1


R.T.: 3.764 min
Delta R.T.: 0.000 min
Response: 121017337
Conc: 525.21 ng/ml

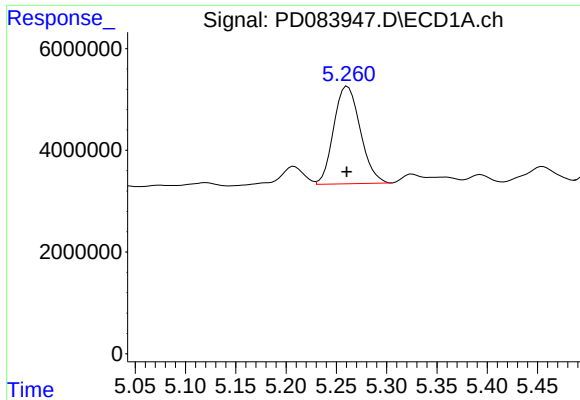

#24 Chlordane-2


R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 35172609
Conc: 517.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071524

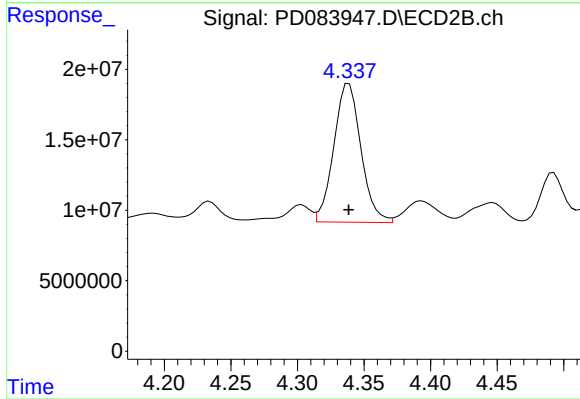


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 139622548
Conc: 521.75 ng/ml

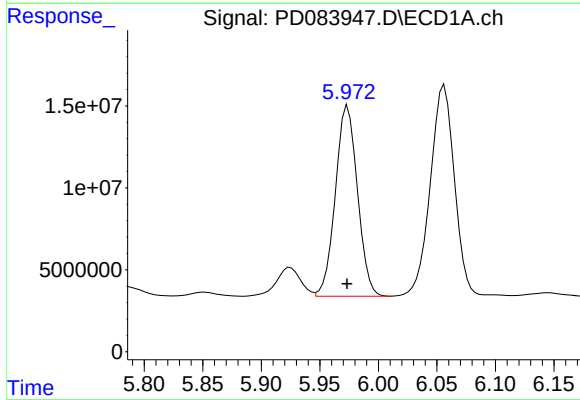


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 152719607
Conc: 518.98 ng/ml

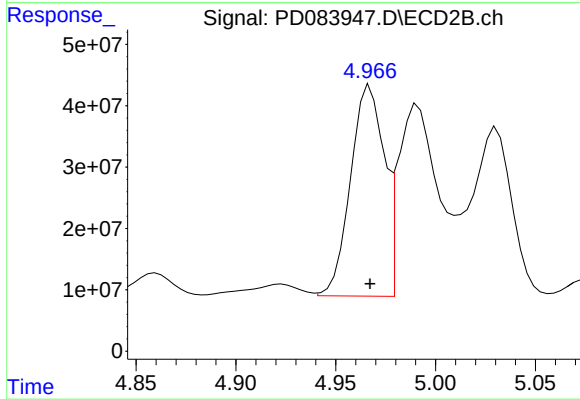

#25 Chlordane-3


R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 400516019
Conc: 524.43 ng/ml

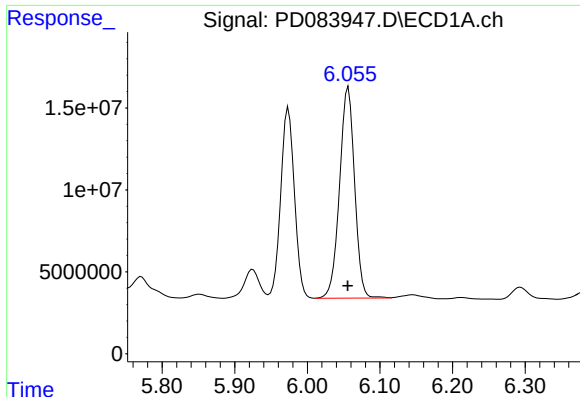

#26 Chlordane-4


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 185470826
Conc: 519.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071524

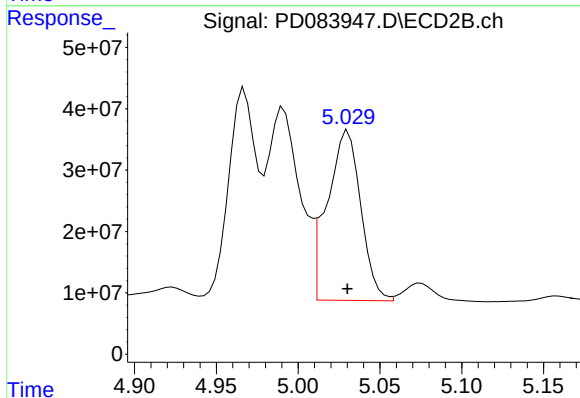


#26 Chlordane-4

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 394780102
Conc: 525.03 ng/ml

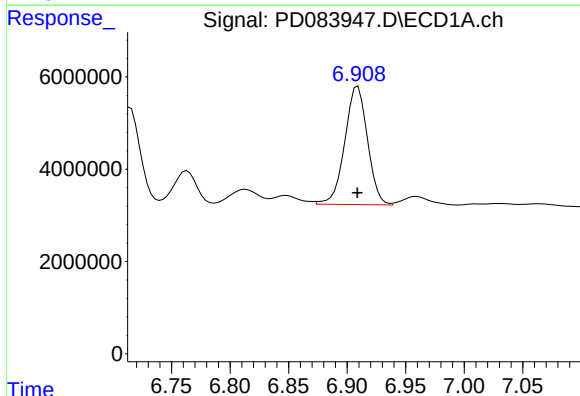


#27 Chlordane-5

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 34601387
Conc: 513.71 ng/ml

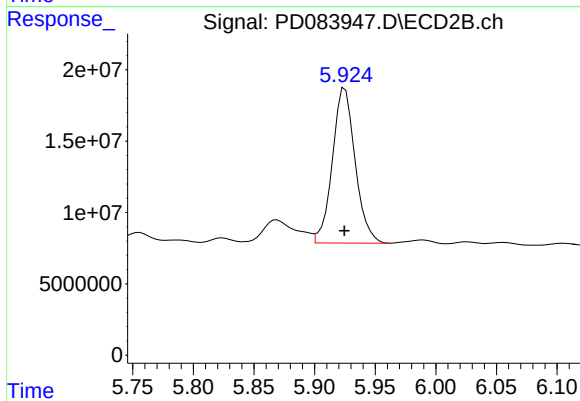

#27 Chlordane-5


R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 141948026
Conc: 519.10 ng/ml

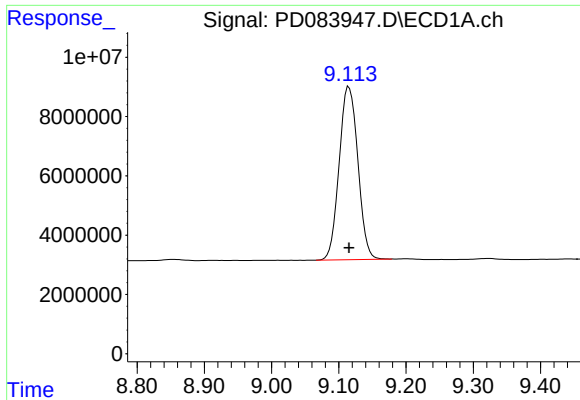

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 112511357
Conc: 51.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071524

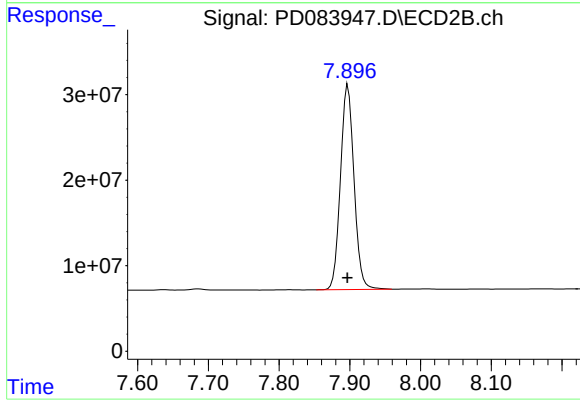

#28 Decachlorobiphenyl

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 319095069
Conc: 51.87 ng/ml