

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD071618\
 Data File : PD048432.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jul 2018 3:21
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 04:06:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071618.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 17 02:42:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.393	4.006	22720011	355.3E6	18.649	19.097
28)	SA Decachlor...	8.084	9.052	29059147	396.7E6	20.264	21.106
Target Compounds							
2)	A alpha-BHC	0.000	4.435f	0	76312945	N.D.	2.509 #
3)	MA gamma-BHC...	4.102	4.635f	4625877	10643041	2.363	0.398 #
6)	B beta-BHC	4.311f	0.000	3275238	0	4.416	N.D. #
8)	B Heptachlo...	0.000	5.860	0	63553998	N.D.	3.154 #
12)	B 4,4'-DDE	0.000	6.389f	0	26030862	N.D.	1.120 #
14)	MA Endrin	5.917	0.000	1764142	0	1.077	N.D. #
16)	A 4,4'-DDD	0.000	6.773f	0	17700380	N.D.	0.900 #
23)	Chlordane-1	4.311	0.000	3275238	0	55.282	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD071618\
Data File : PD048432.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jul 2018 3:21
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 04:06:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071618.M
Quant Title : GC Extractables
QLast Update : Tue Jul 17 02:42:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

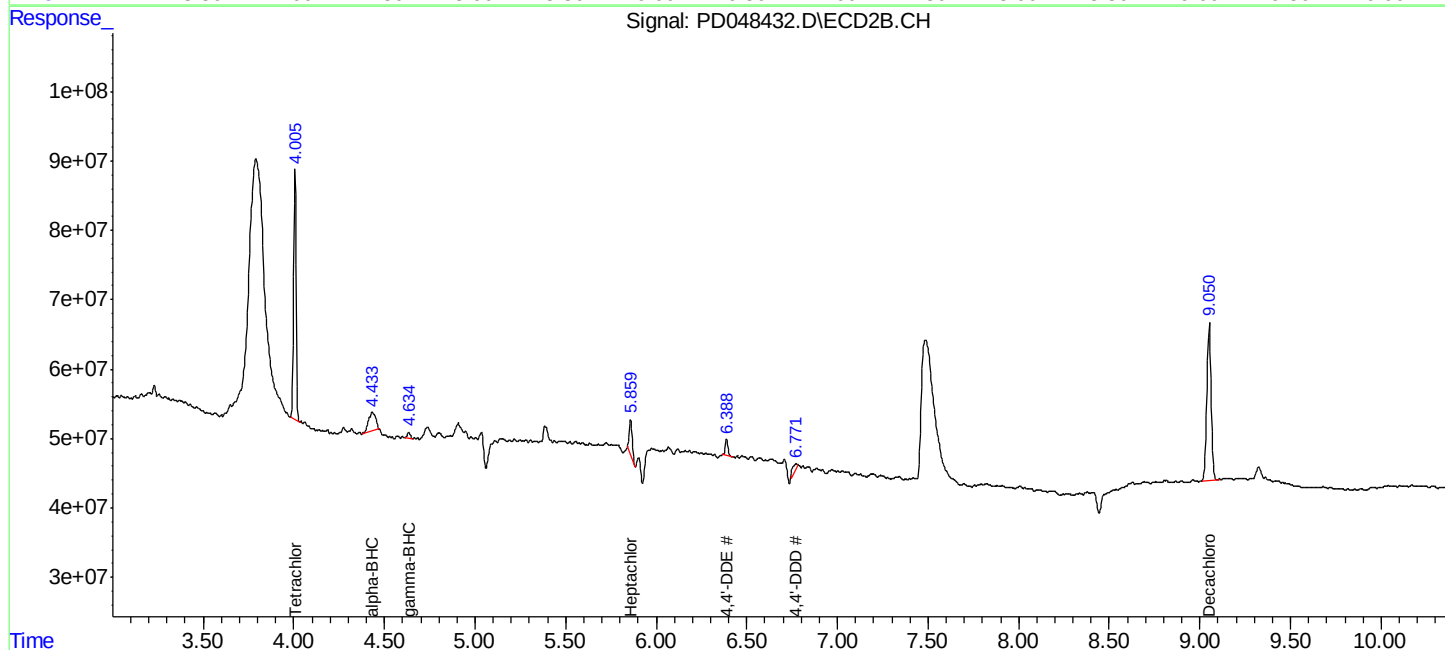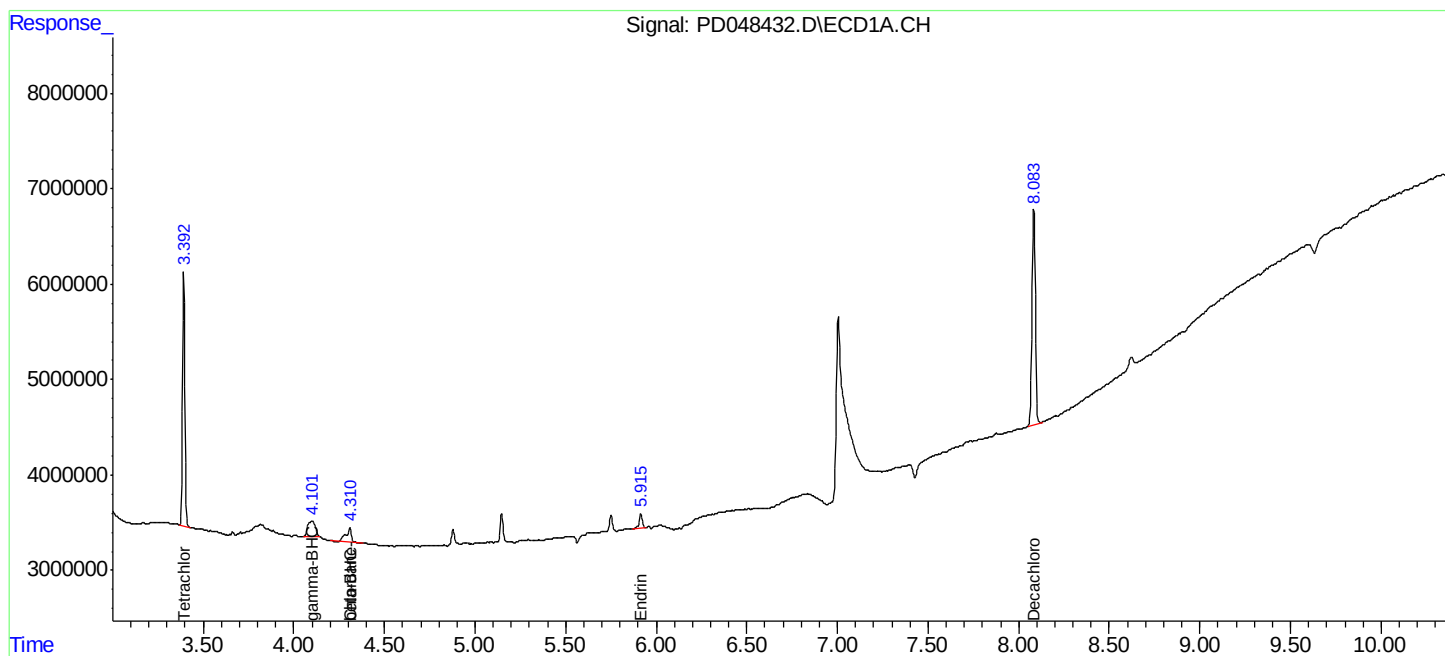


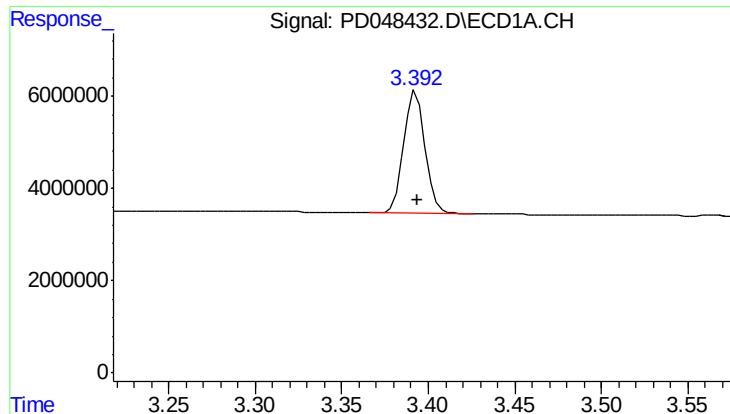

#1 Tetrachloro-m-xylene


R.T.: 3.393 min
Delta R.T.: 0.000 min
Response: 22720011
Conc: 18.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

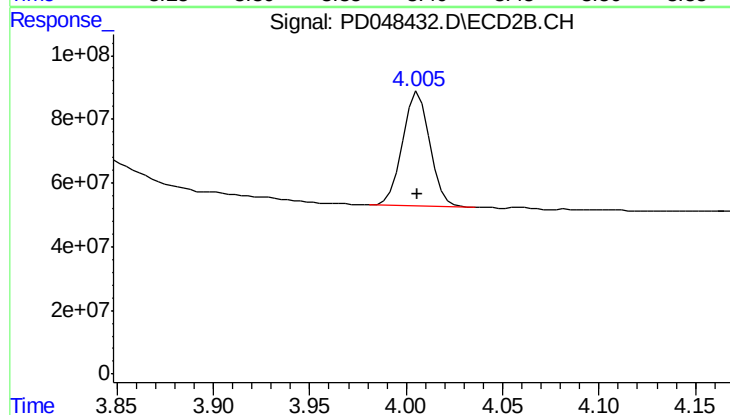


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 355256590
Conc: 19.10 ng/ml

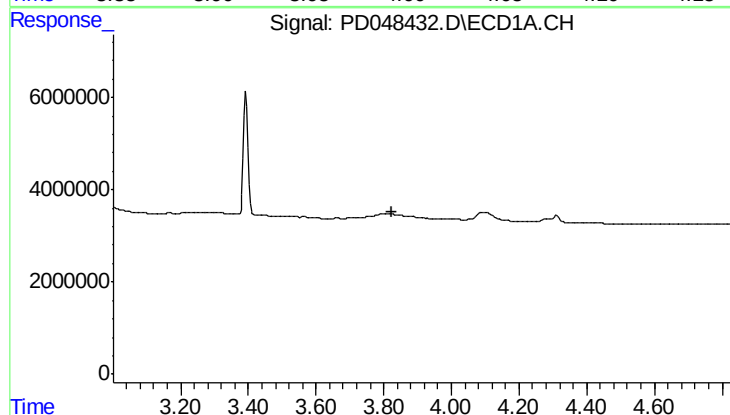


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 3.826 min
Response: 0
Conc: N.D.

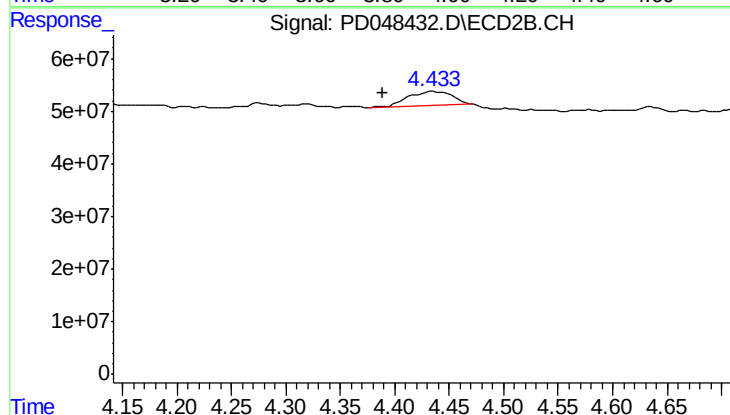

#2 alpha-BHC


R.T.: 4.435 min
Delta R.T.: 0.045 min
Response: 76312945
Conc: 2.51 ng/ml

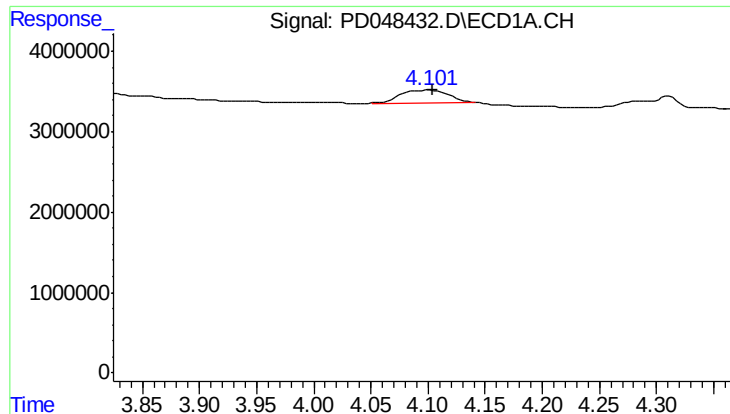

#3 gamma-BHC (Lindane)


R.T.: 4.102 min
Delta R.T.: -0.002 min
Response: 4625877
Conc: 2.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

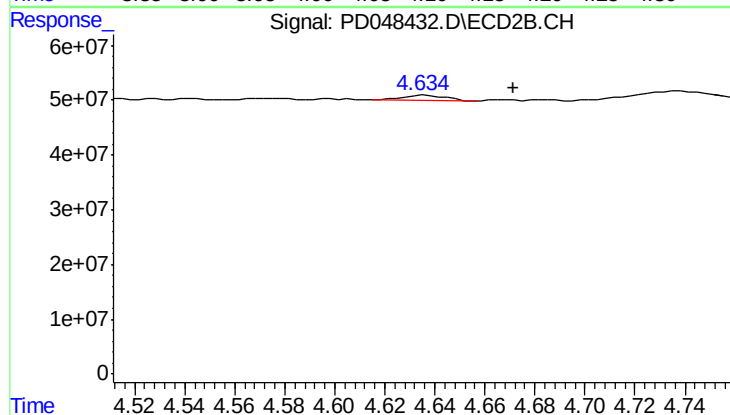


#3 gamma-BHC (Lindane)

R.T.: 4.635 min
Delta R.T.: -0.036 min
Response: 10643041
Conc: 0.40 ng/ml

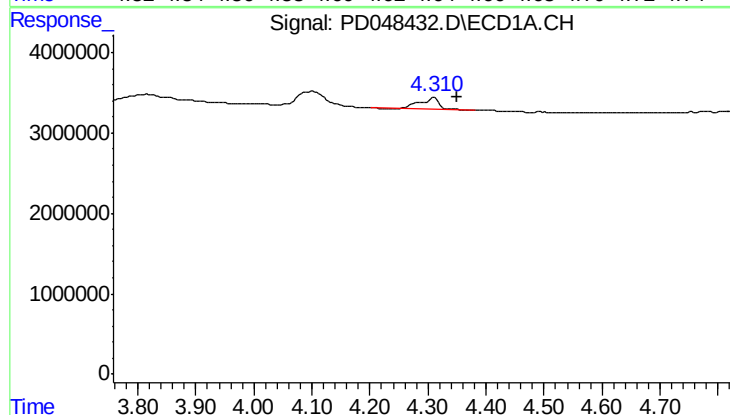


#6 beta-BHC

R.T.: 4.311 min
Delta R.T.: -0.039 min
Response: 3275238
Conc: 4.42 ng/ml

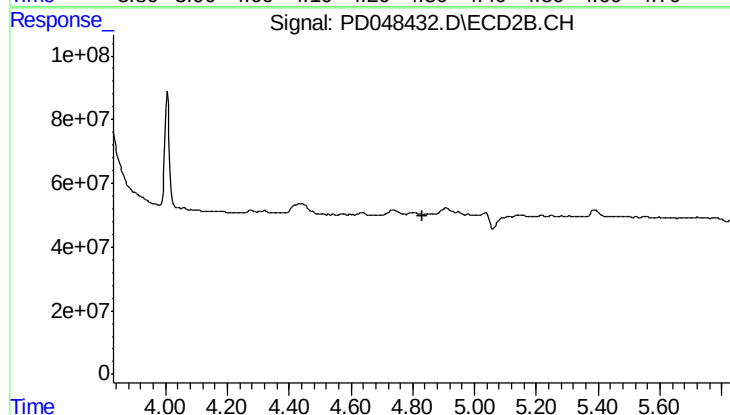

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.831 min
Response: 0
Conc: N.D.

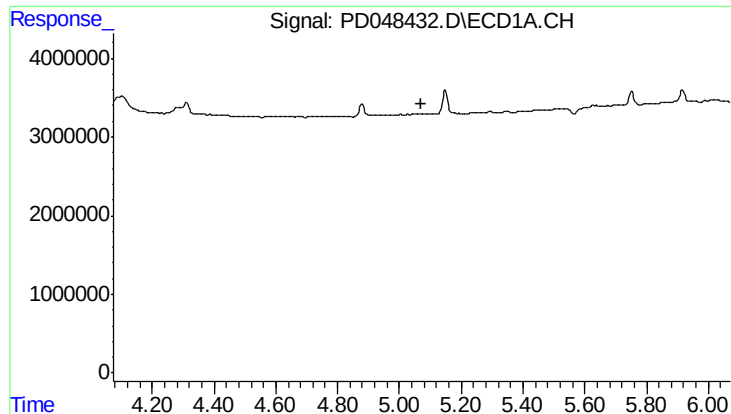

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

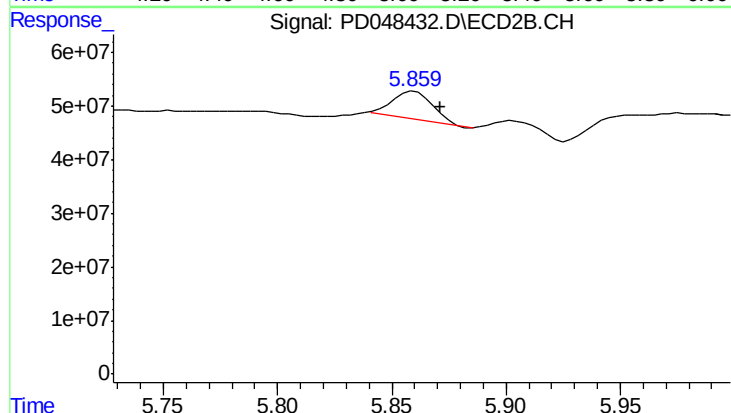


#8 Heptachlor epoxide

R.T.: 5.860 min
Delta R.T.: -0.011 min
Response: 63553998
Conc: 3.15 ng/ml

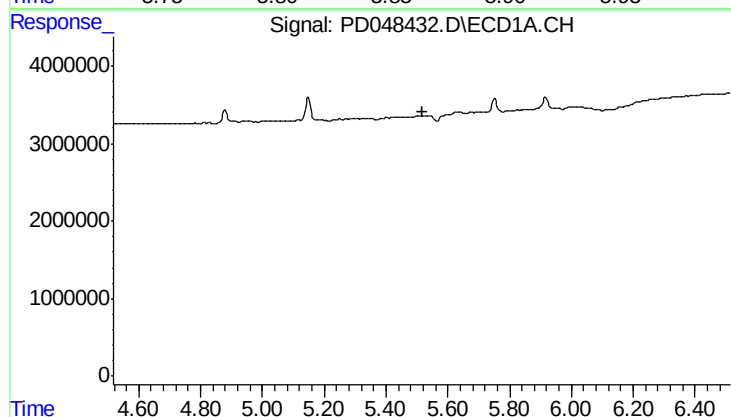


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

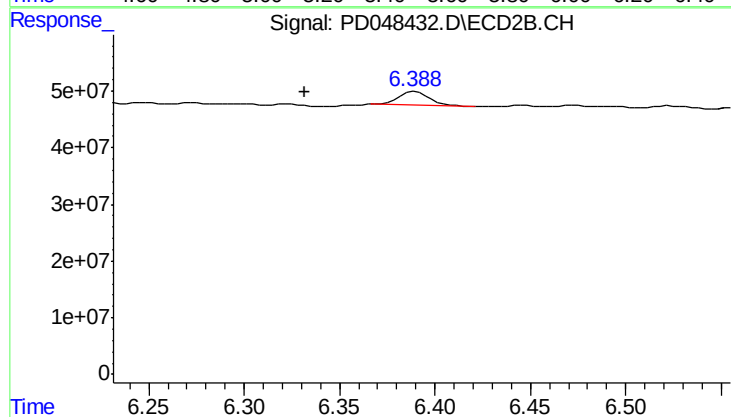

#12 4,4'-DDE


R.T.: 6.389 min
Delta R.T.: 0.058 min
Response: 26030862
Conc: 1.12 ng/ml

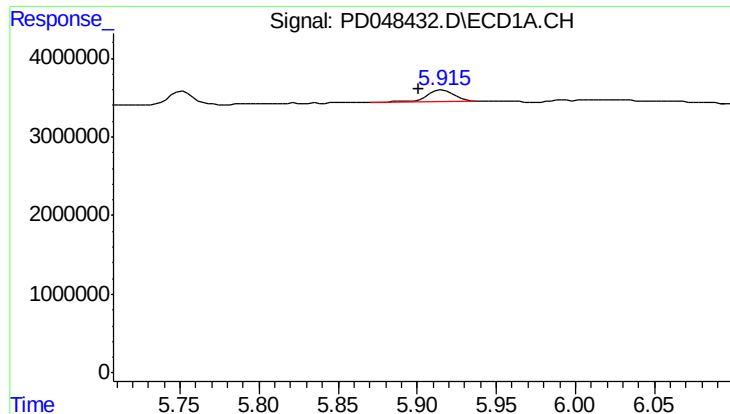

#14 Endrin


R.T.: 5.917 min
Delta R.T.: 0.016 min
Response: 1764142
Conc: 1.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

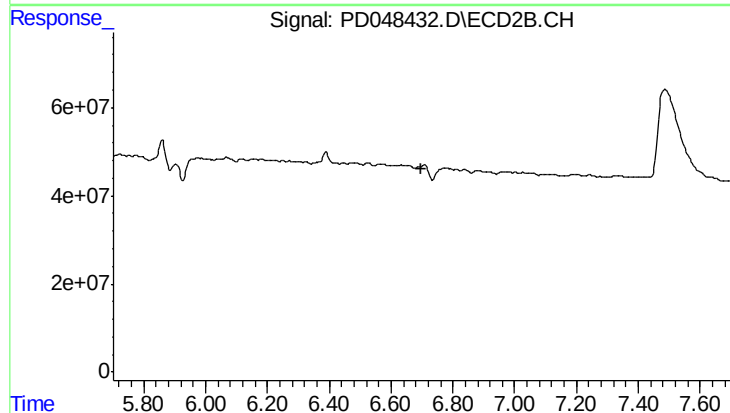


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.698 min
Response: 0
Conc: N.D.

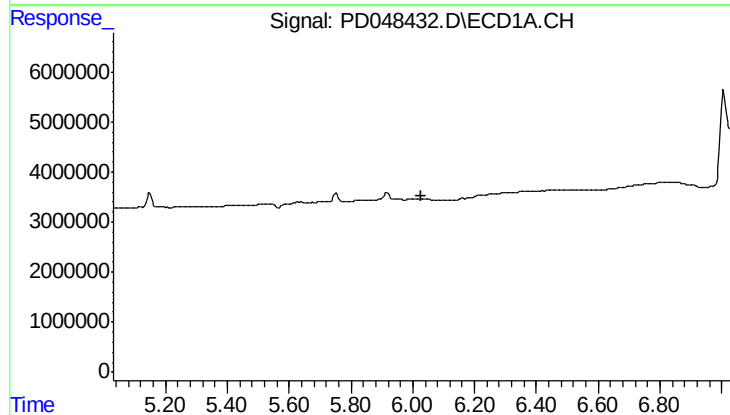


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.029 min
Response: 0
Conc: N.D.

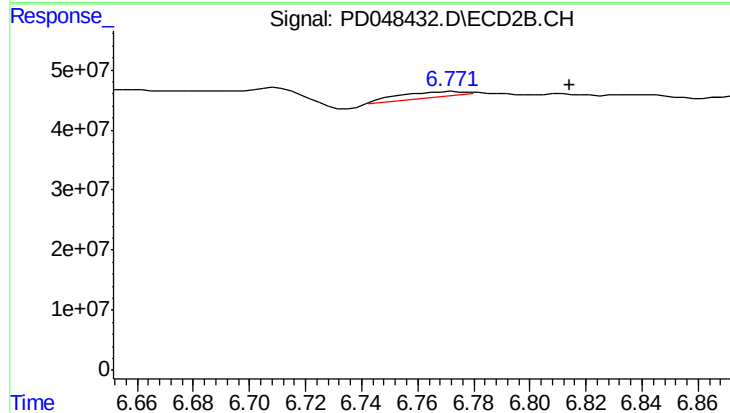

#16 4,4'-DDD


R.T.: 6.773 min
Delta R.T.: -0.041 min
Response: 17700380
Conc: 0.90 ng/ml

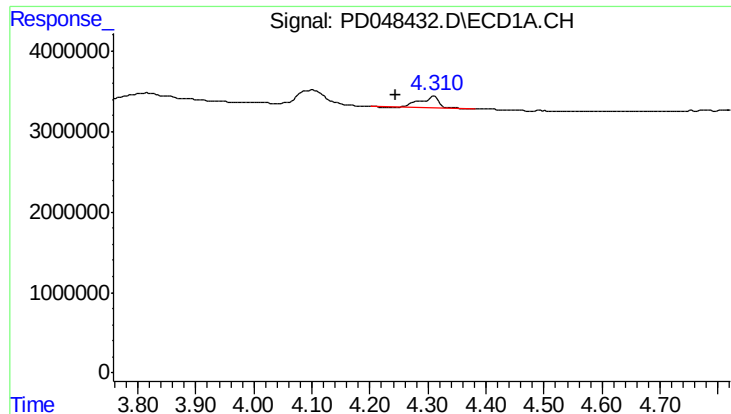

#23 Chlordane-1


R.T.: 4.311 min
Delta R.T.: 0.066 min
Response: 3275238
Conc: 55.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

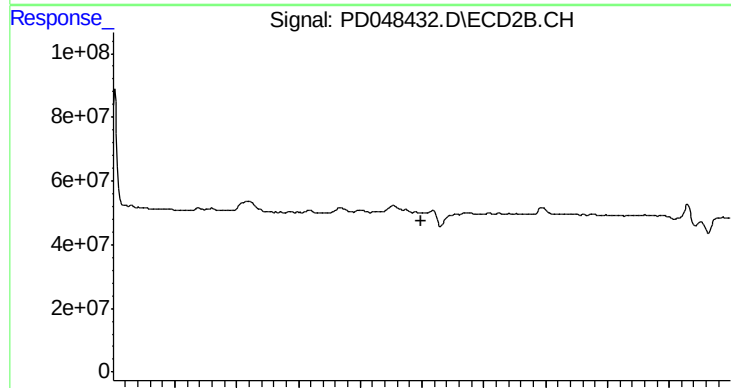


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.998 min
Response: 0
Conc: N.D.

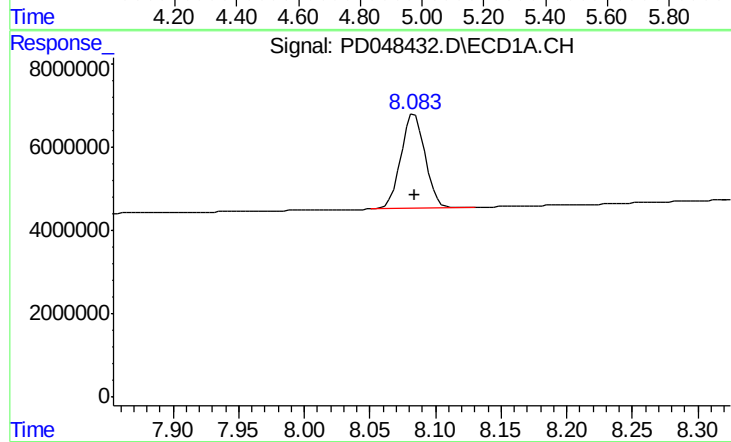

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 29059147
Conc: 20.26 ng/ml

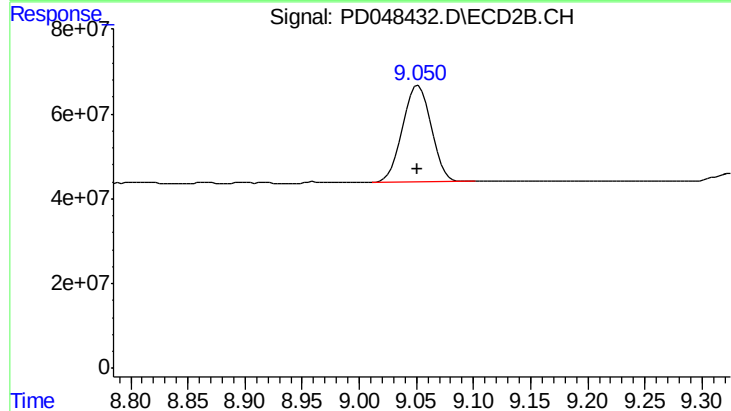

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: 0.000 min
Response: 396650315
Conc: 21.11 ng/ml