

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 09:04
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:45:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA gamma-BHC...	0.000	4.532	0	441024	N.D.	0.128 #
--------------------	-------	-------	---	--------	------	---------



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 09:04
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:45:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

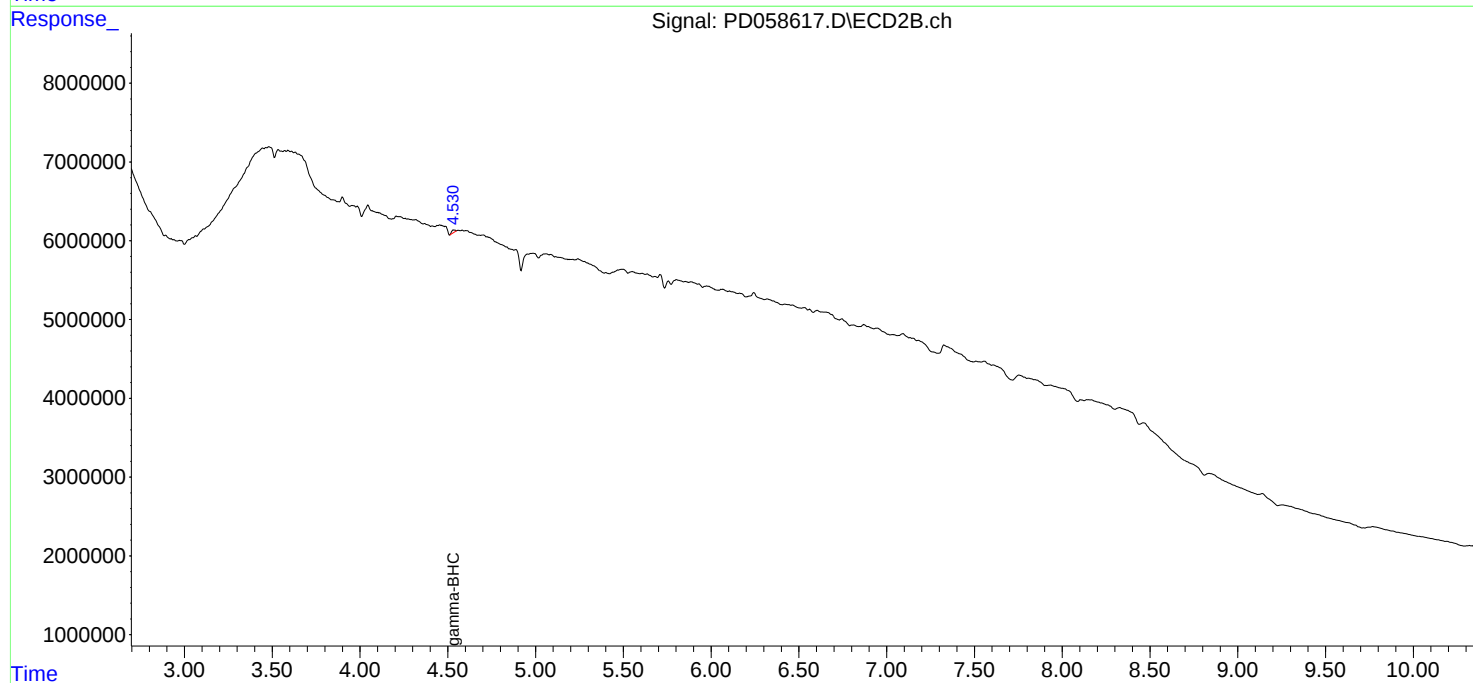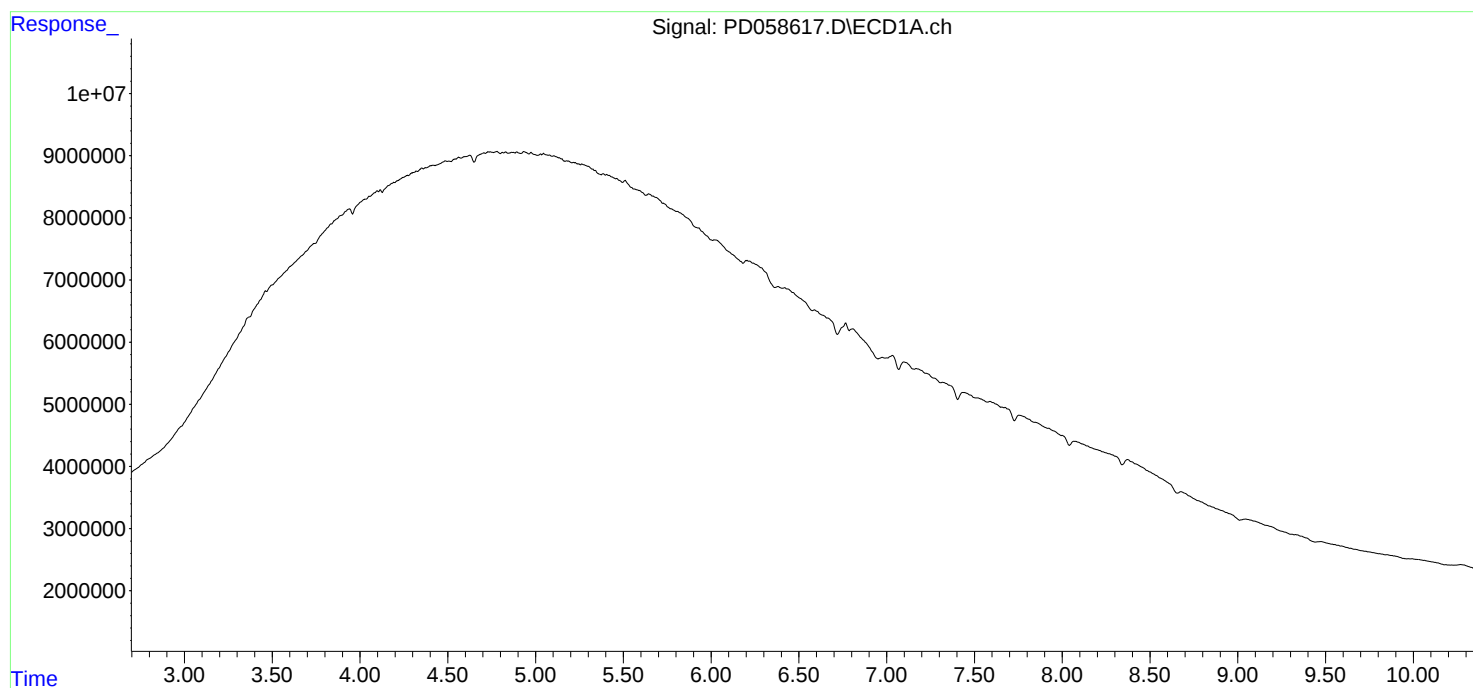


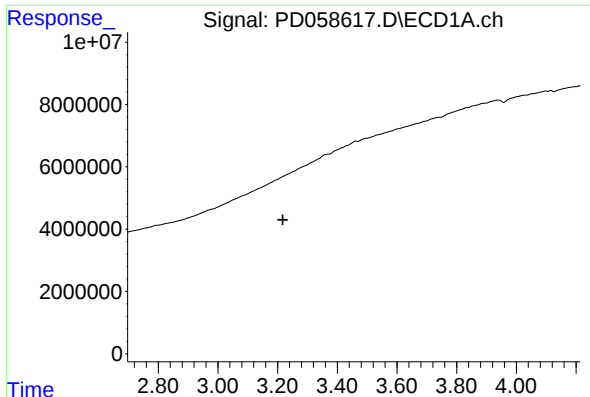

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

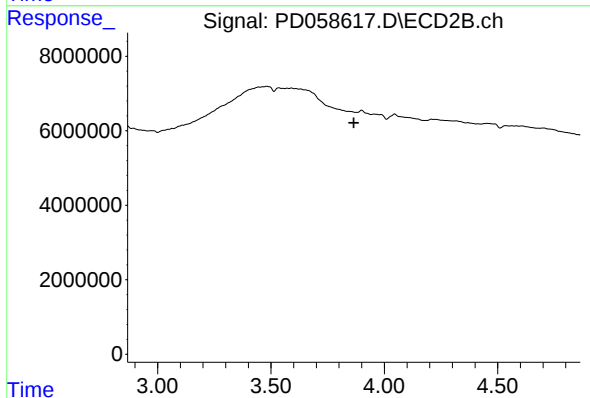


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.866 min
Response: 0
Conc: N.D.

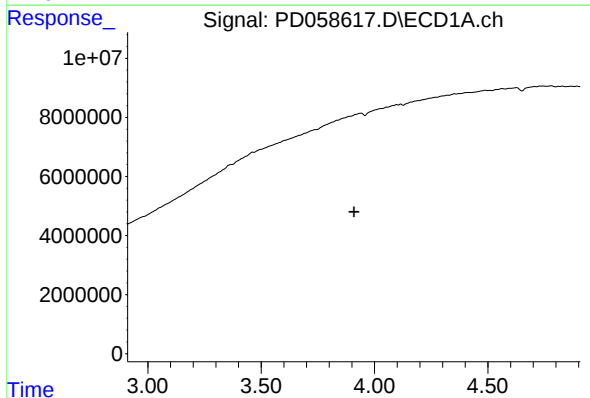


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

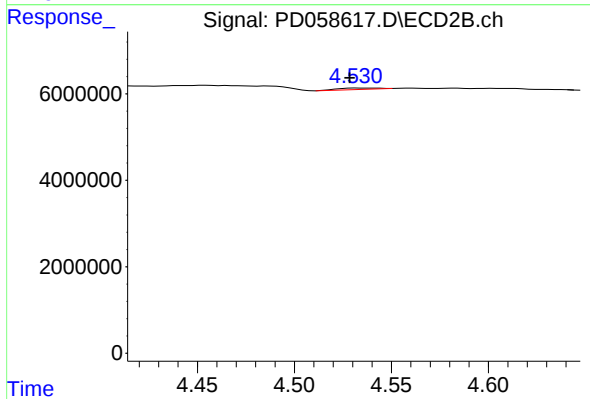

#3 gamma-BHC (Lindane)


R.T.: 4.532 min
Delta R.T.: 0.003 min
Response: 441024
Conc: 0.13 ng/ml

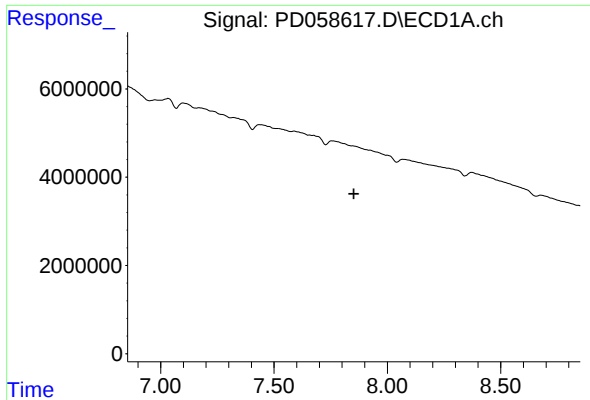

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

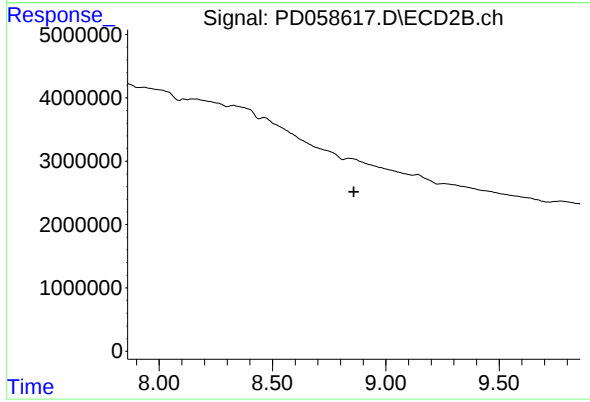

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.859 min
Response: 0
Conc: N.D.