

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 11:34
 Operator : AJ\MA
 Sample : L3300-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-8A-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:48:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	24763248	34582021	13.581	13.996
28)	SA Decachlor...	7.844	8.858	26007530	33174178	14.402	15.216
Target Compounds							
8)	B Heptachlo...	0.000	5.709	0	10464474	N.D.	3.595 #
9)	A Endosulfan I	0.000	6.057	0	1255029	N.D.	0.476 #
10)	B gamma-Chl...	0.000	5.934	0	4503887	N.D.	1.548 #
11)	B alpha-Chl...	0.000	6.018	0	5751093	N.D.	2.000 #
15)	B Endosulfa...	0.000	6.770f	0	880685	N.D.	0.357 #
25)	Chlordane-3	0.000	5.934	0	4503887	N.D.	12.109 #
26)	Chlordane-4	0.000	6.018	0	5751093	N.D.	13.221 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 11:34
Operator : AJ\MA
Sample : L3300-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
TP-8A-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:48:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

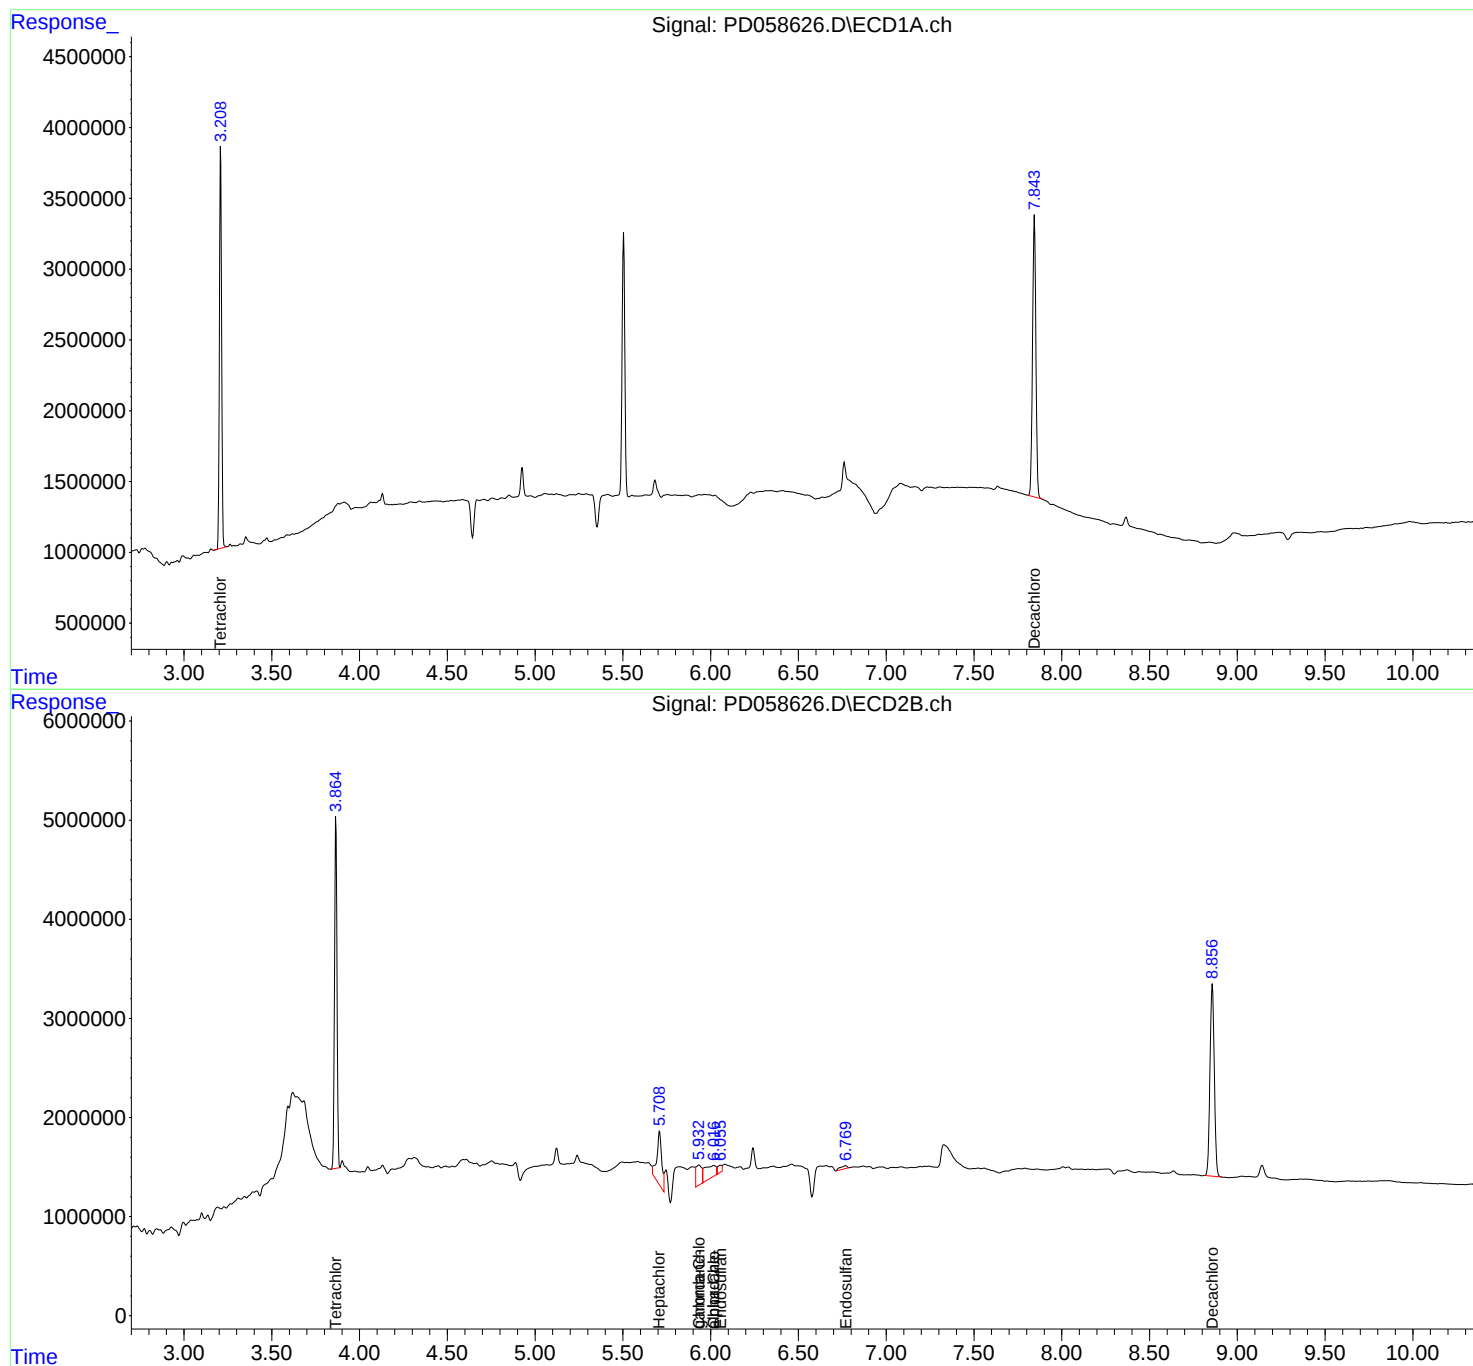


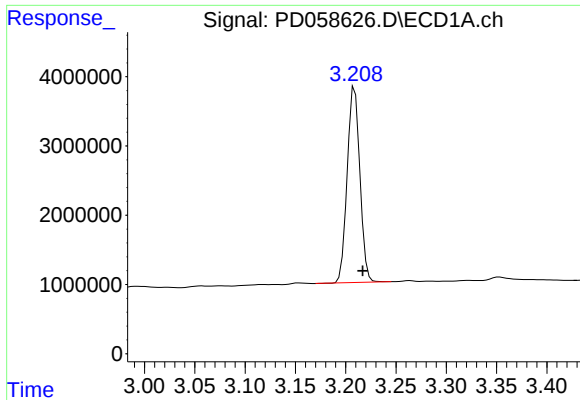

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 24763248
Conc: 13.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8A-S

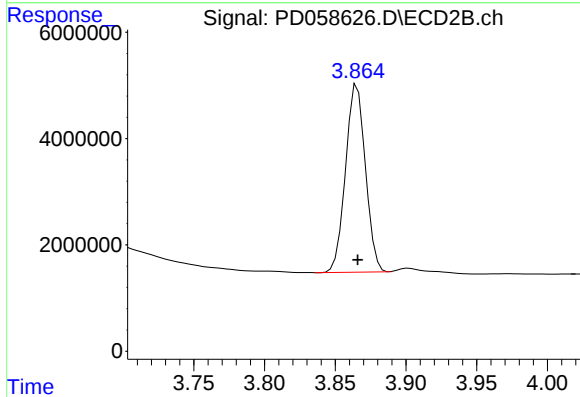


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 34582021
Conc: 14.00 ng/ml

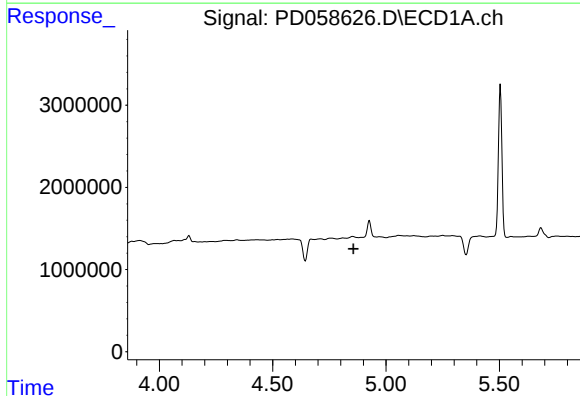


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

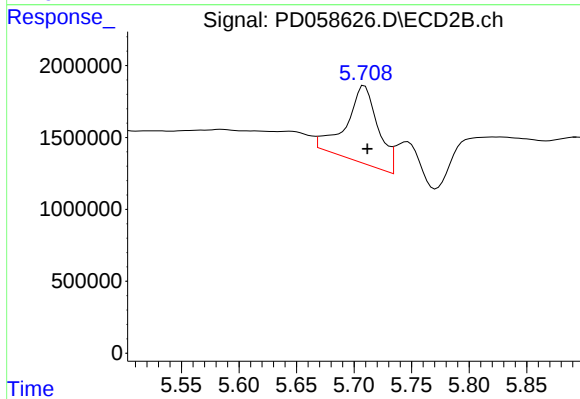

#8 Heptachlor epoxide


R.T.: 5.709 min
Delta R.T.: -0.002 min
Response: 10464474
Conc: 3.59 ng/ml

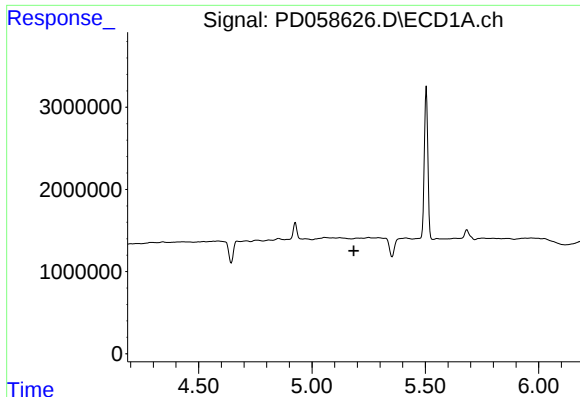

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-8A-S

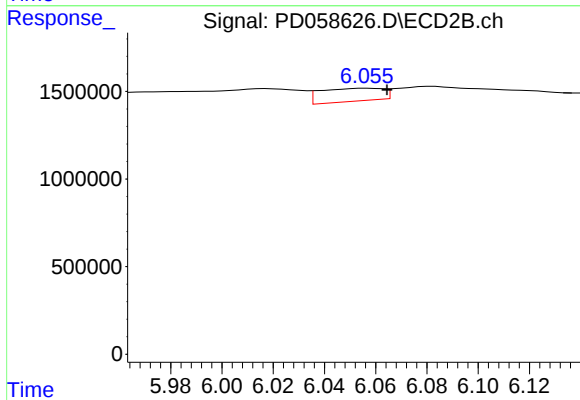


#9 Endosulfan I

R.T.: 6.057 min
Delta R.T.: -0.008 min
Response: 1255029
Conc: 0.48 ng/ml

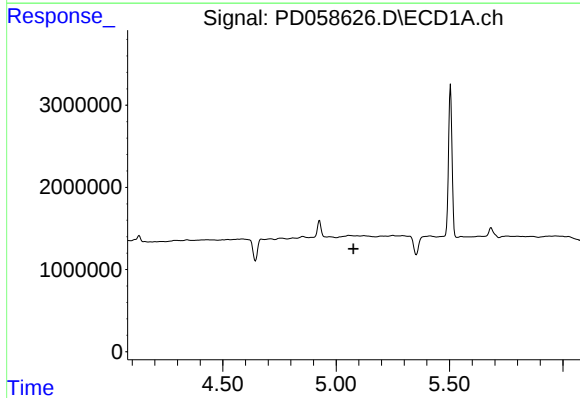


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

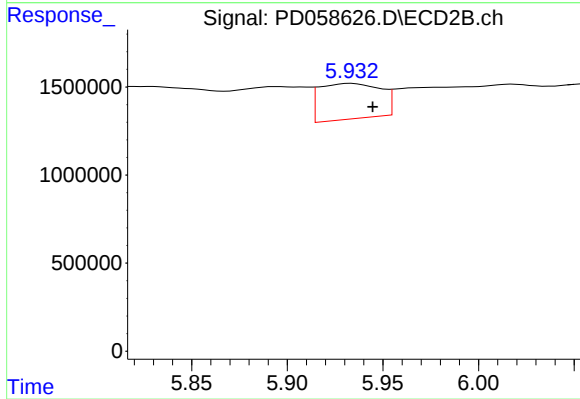

#10 gamma-Chlordane


R.T.: 5.934 min
Delta R.T.: -0.011 min
Response: 4503887
Conc: 1.55 ng/ml

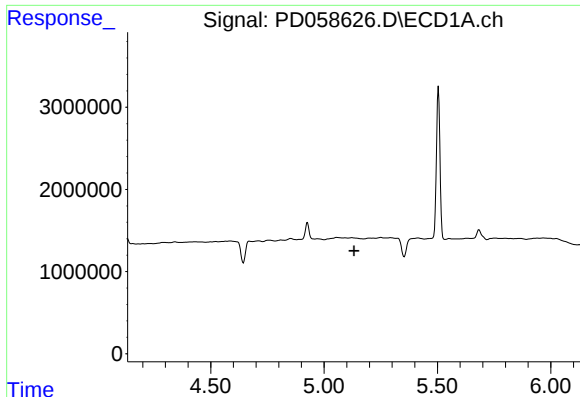

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-8A-S

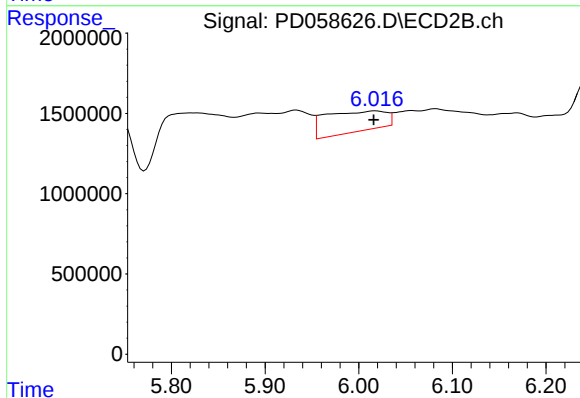


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.002 min
Response: 5751093
Conc: 2.00 ng/ml

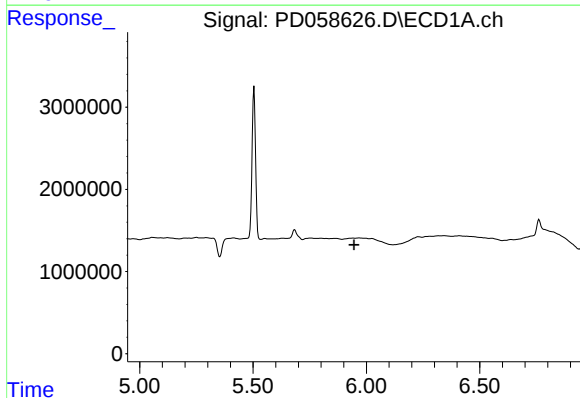


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.946 min
Response: 0
Conc: N.D.

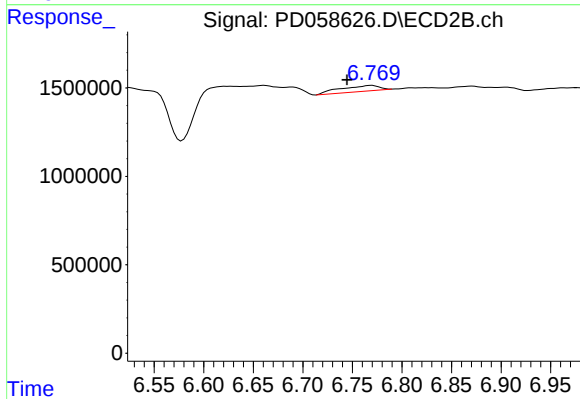

#15 Endosulfan II


R.T.: 6.770 min
Delta R.T.: 0.025 min
Response: 880685
Conc: 0.36 ng/ml

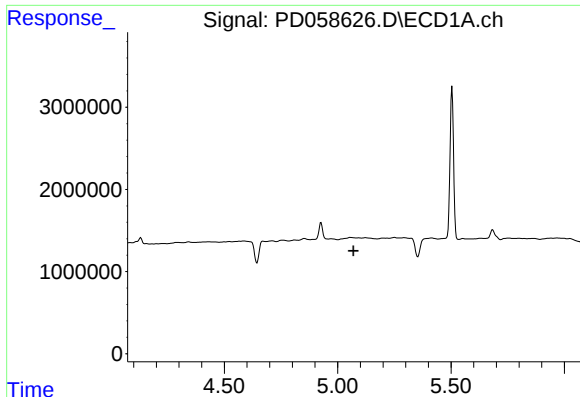

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-8A-S

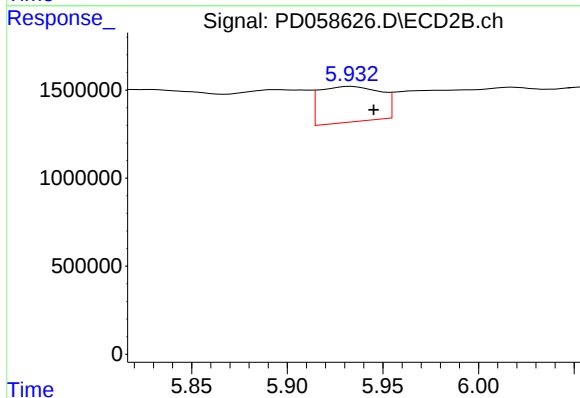


#25 Chlordane-3

R.T.: 5.934 min
Delta R.T.: -0.012 min
Response: 4503887
Conc: 12.11 ng/ml

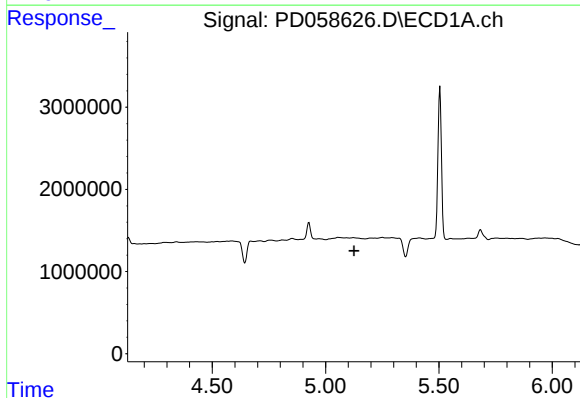


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

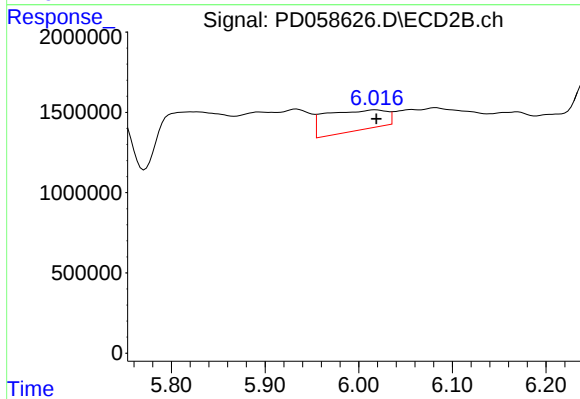

#26 Chlordane-4


R.T.: 6.018 min
Delta R.T.: -0.001 min
Response: 5751093
Conc: 13.22 ng/ml

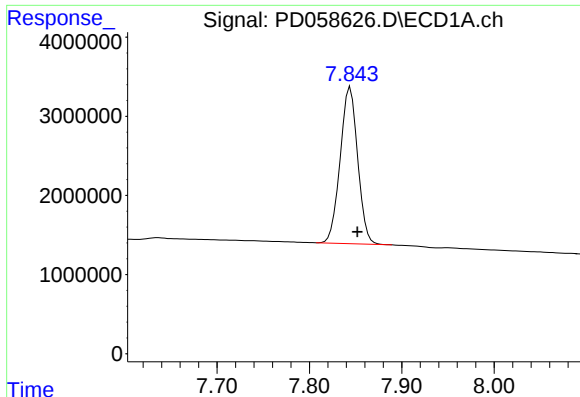

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 26007530
Conc: 14.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8A-S

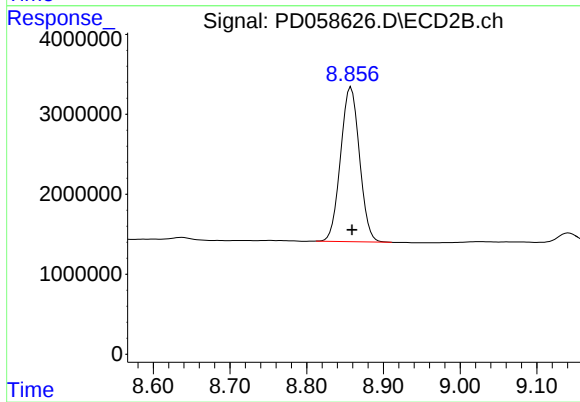

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: -0.002 min
Response: 33174178
Conc: 15.22 ng/ml