

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 11:49
 Operator : AJ\MA
 Sample : L3300-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-8A-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:48:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.865	20210681	26461780	11.085	10.710
28)	SA Decachlor...	7.843	8.857	19453422	26691435	10.772	12.242
Target Compounds							
2)	A alpha-BHC	0.000	4.274f	0	1720031	N.D.	0.456 #
8)	B Heptachlo...	0.000	5.709	0	20769701	N.D.	7.135 #
9)	A Endosulfan I	0.000	6.080f	0	2128884	N.D.	0.807 #
10)	B gamma-Chl...	0.000	5.937	0	12929412	N.D.	4.443 #
11)	B alpha-Chl...	0.000	6.017	0	6648735	N.D.	2.312 #
14)	MA Endrin	5.683	0.000	10048333	0	7.056	N.D. #
25)	Chlordane-3	0.000	5.937	0	12929412	N.D.	34.762 #
26)	Chlordane-4	0.000	6.017	0	6648735	N.D.	15.284 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 11:49
Operator : AJ\MA
Sample : L3300-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-8A-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:48:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

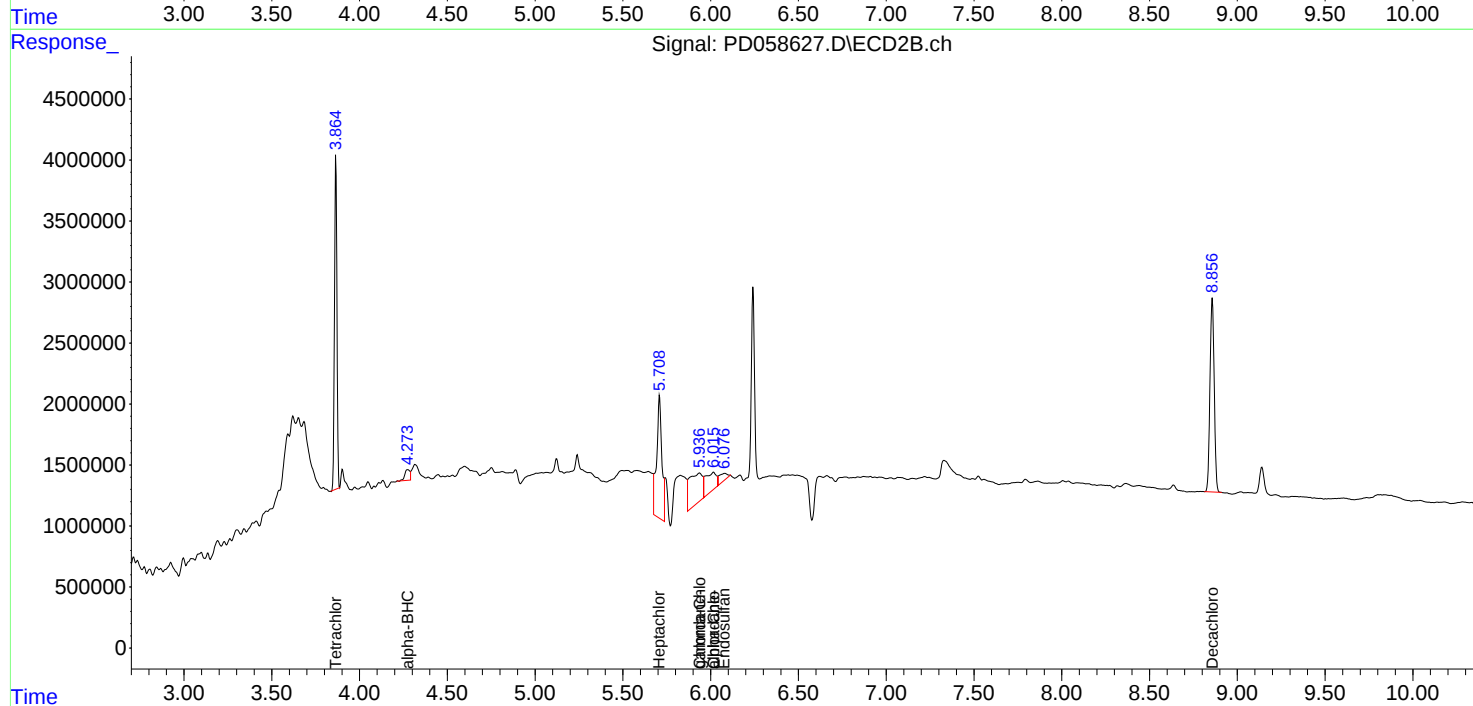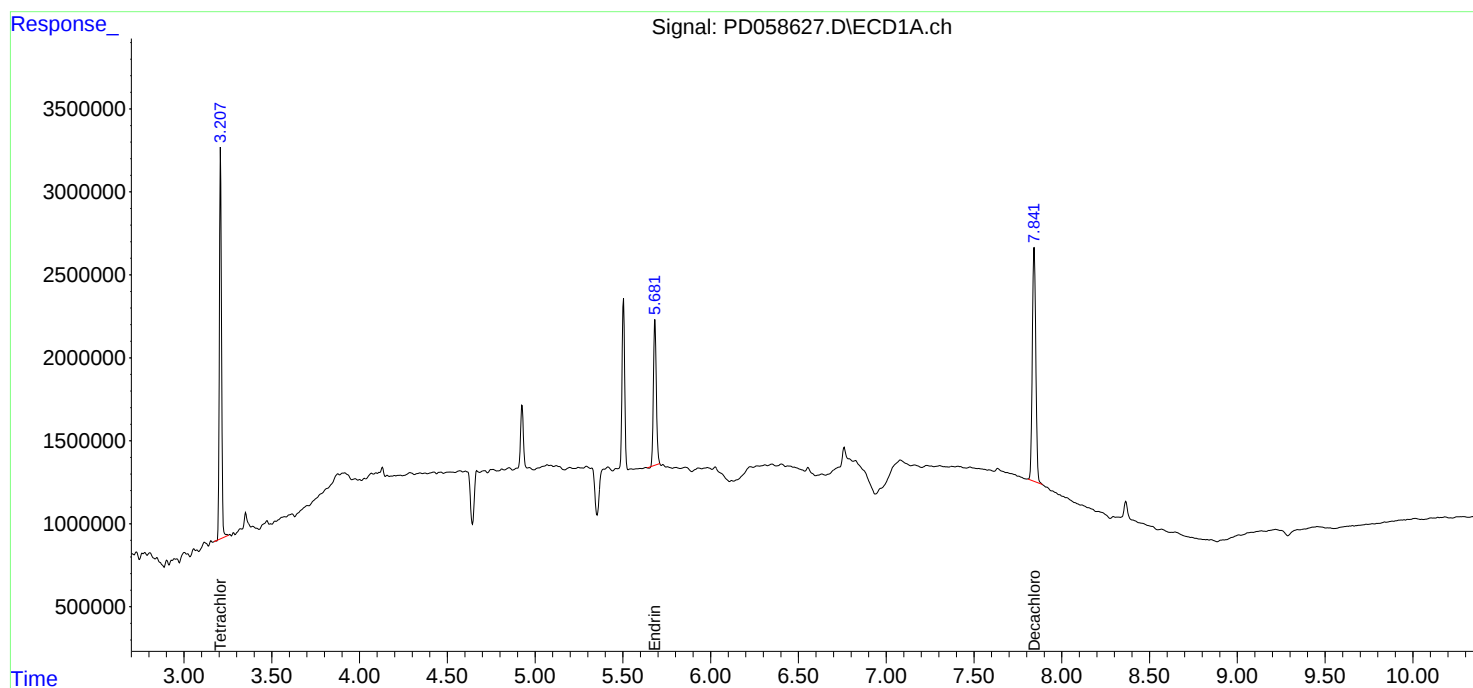


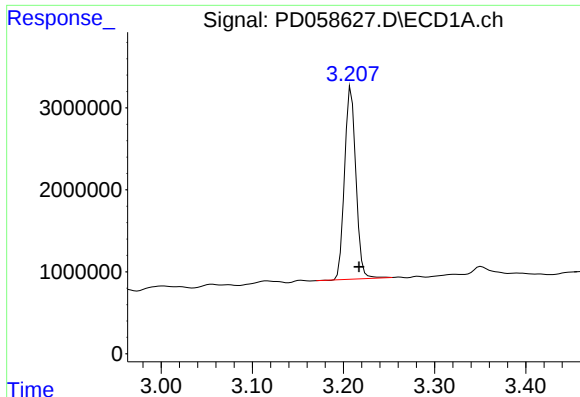

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 20210681
Conc: 11.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8A-D

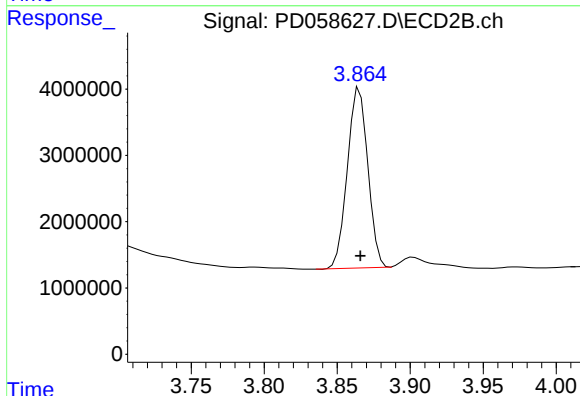


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 26461780
Conc: 10.71 ng/ml

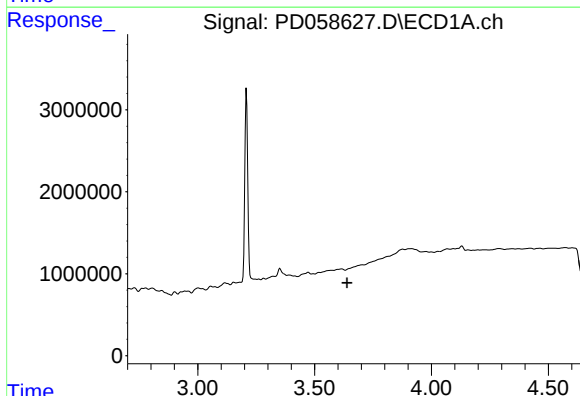


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.639 min
Response: 0
Conc: N.D.

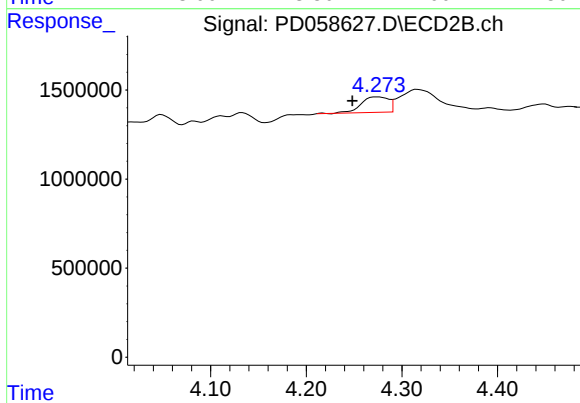

#2 alpha-BHC


R.T.: 4.274 min
Delta R.T.: 0.026 min
Response: 1720031
Conc: 0.46 ng/ml

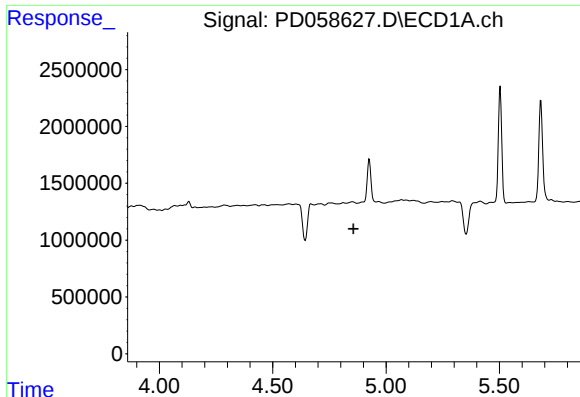

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-8A-D

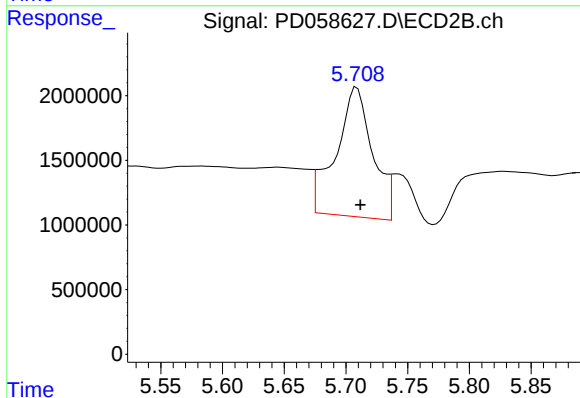


#8 Heptachlor epoxide

R.T.: 5.709 min
Delta R.T.: -0.003 min
Response: 20769701
Conc: 7.13 ng/ml

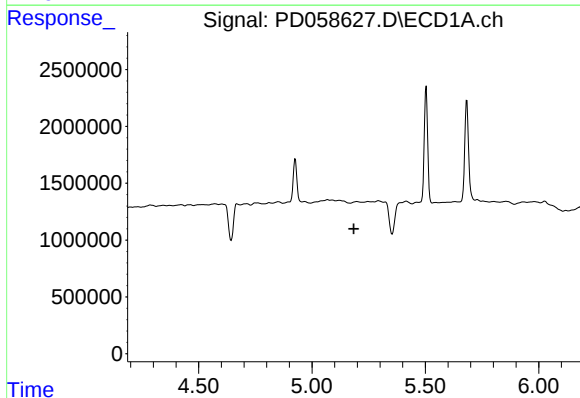


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

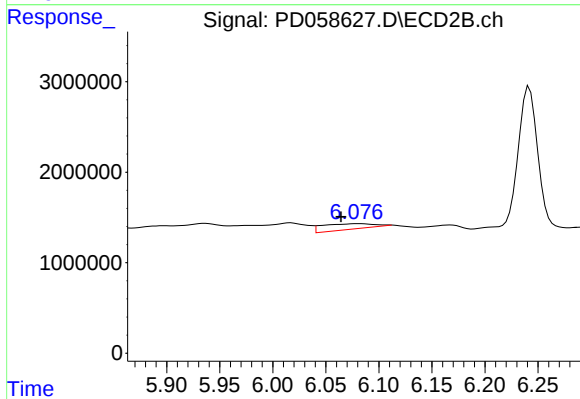

#9 Endosulfan I


R.T.: 6.080 min
Delta R.T.: 0.015 min
Response: 2128884
Conc: 0.81 ng/ml

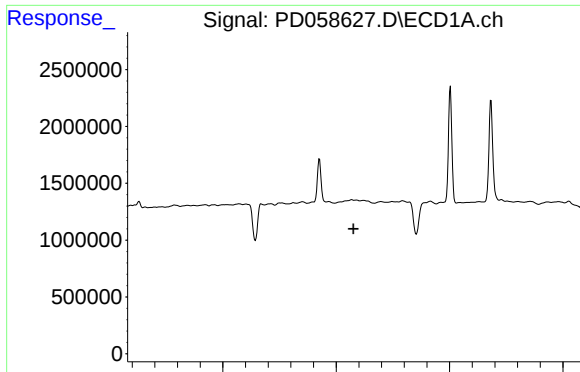

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-8A-D

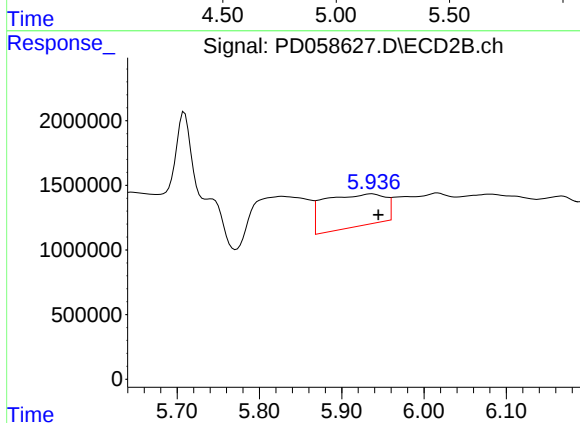


#10 gamma-Chlordane

R.T.: 5.937 min
Delta R.T.: -0.008 min
Response: 12929412
Conc: 4.44 ng/ml

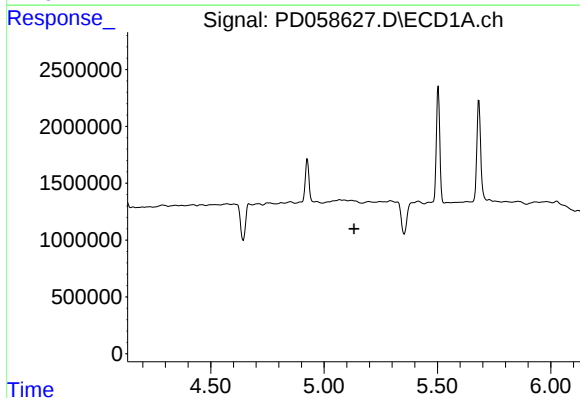


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

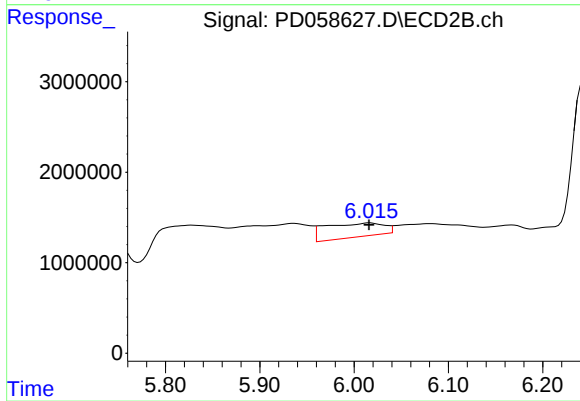

#11 alpha-Chlordane


R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 6648735
Conc: 2.31 ng/ml

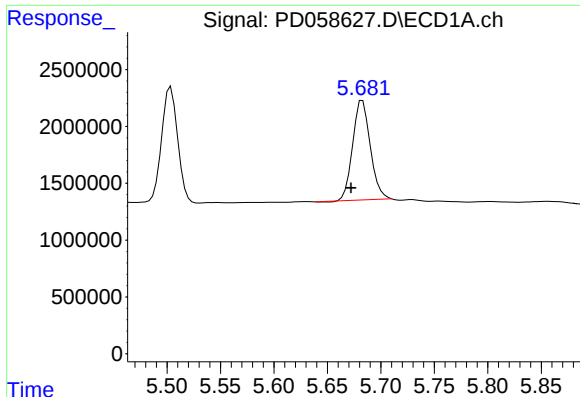

#14 Endrin


R.T.: 5.683 min
Delta R.T.: 0.011 min
Response: 10048333
Conc: 7.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8A-D

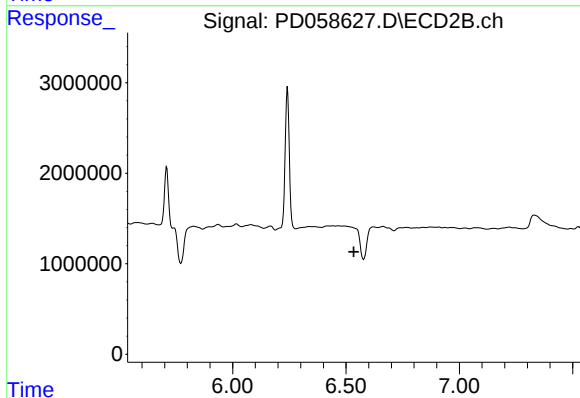


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.535 min
Response: 0
Conc: N.D.

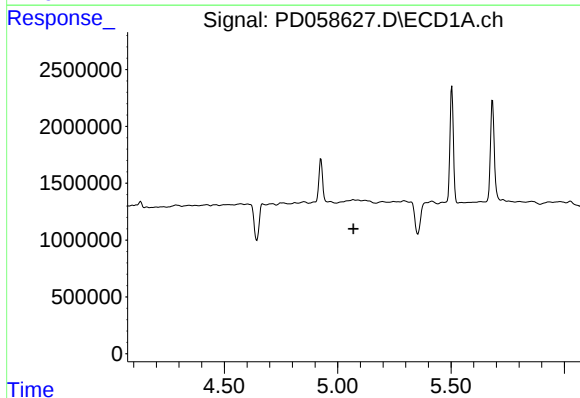


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.070 min
Response: 0
Conc: N.D.

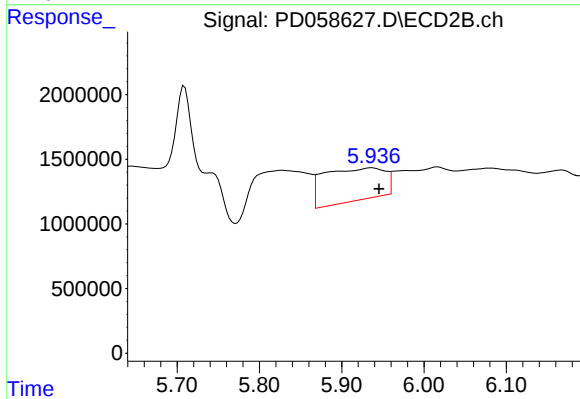

#25 Chlordane-3


R.T.: 5.937 min
Delta R.T.: -0.009 min
Response: 12929412
Conc: 34.76 ng/ml

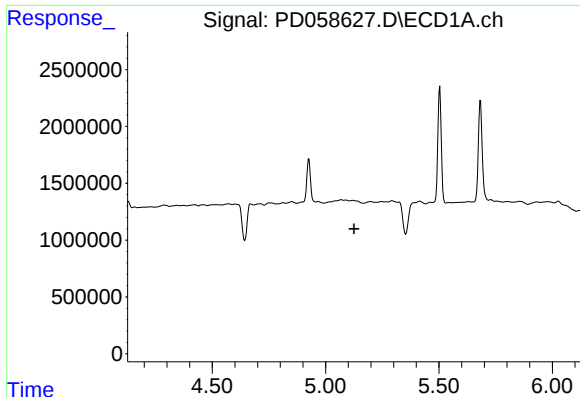

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-8A-D

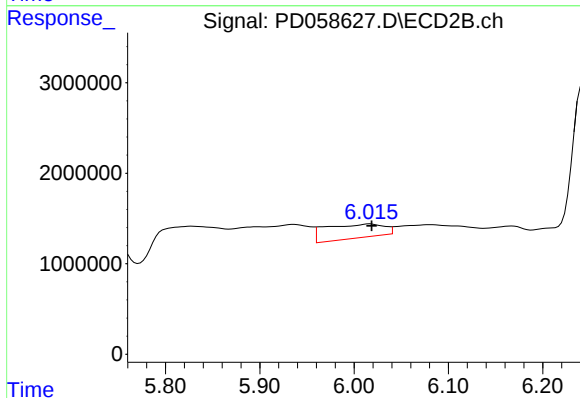


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: -0.002 min
Response: 6648735
Conc: 15.28 ng/ml

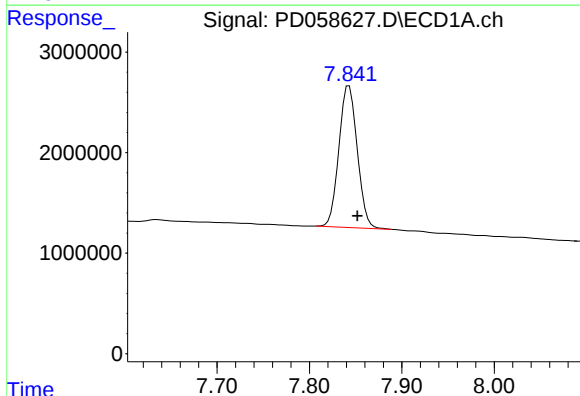

#28 Decachlorobiphenyl

R.T.: 7.843 min
Delta R.T.: -0.009 min
Response: 19453422
Conc: 10.77 ng/ml

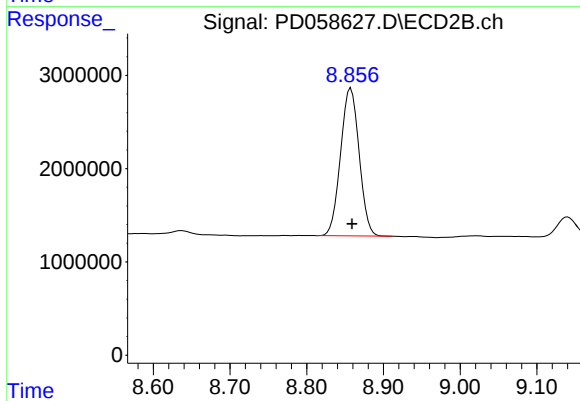

#28 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: -0.002 min
Response: 26691435
Conc: 12.24 ng/ml