

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 13:36
 Operator : AJ\MA
 Sample : L3308-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:49:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.866	22280694	30169655	12.220	12.211
28)	SA Decachlor...	7.845	8.858	14914048	18786221	8.259	8.616
Target Compounds							
2)	A alpha-BHC	0.000	4.277f	0	4045475	N.D.	1.073 #
3)	MA gamma-BHC...	0.000	4.530	0	634685	N.D.	0.184 #
4)	MA Heptachlor	0.000	5.051f	0	485623	N.D.	0.154 #
10)	B gamma-Chl...	0.000	5.944	0	2433593	N.D.	0.836 #
11)	B alpha-Chl...	0.000	6.019	0	4943470	N.D.	1.719 #
12)	B 4,4'-DDE	0.000	6.175	0	952453	N.D.	0.347 #
25)	Chlordane-3	0.000	5.944	0	2433593	N.D.	6.543 #
26)	Chlordane-4	0.000	6.019	0	4943470	N.D.	11.364 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 13:36
Operator : AJ\MA
Sample : L3308-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:49:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

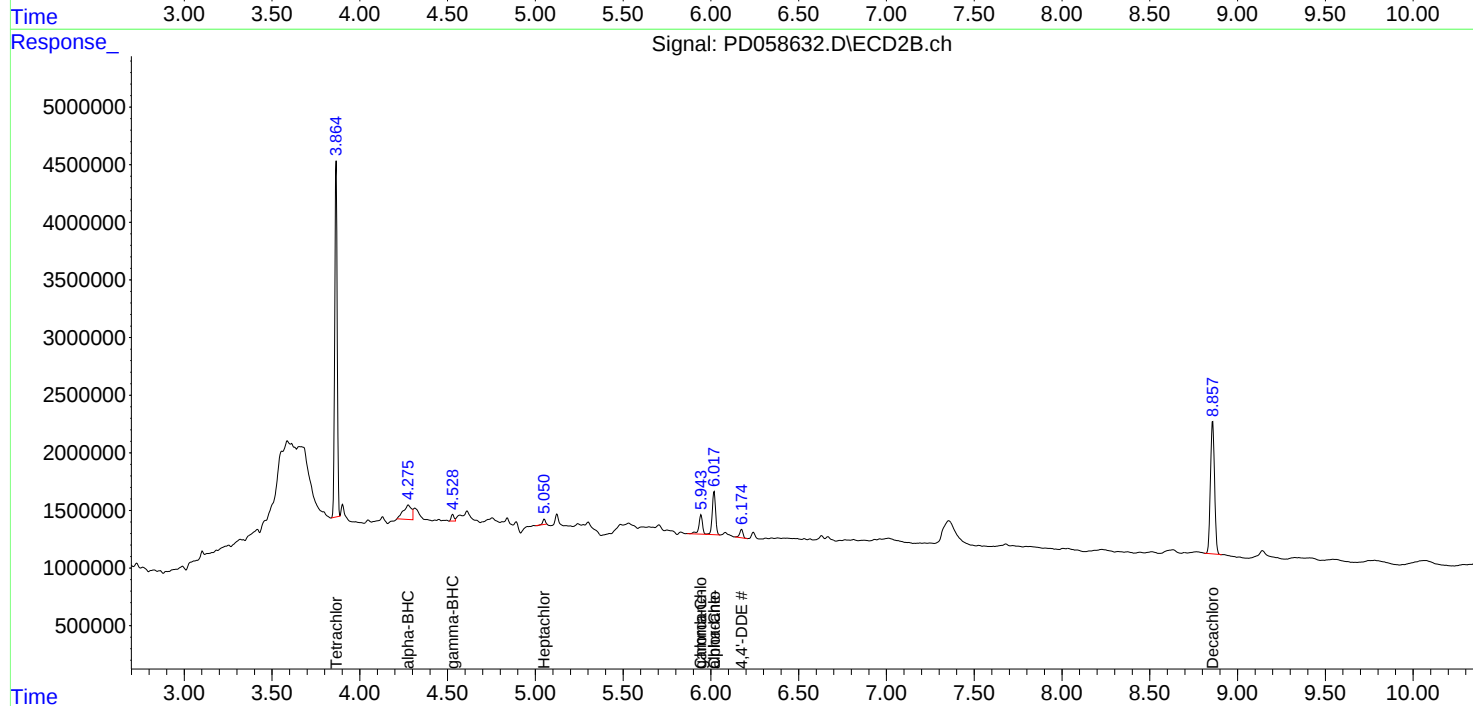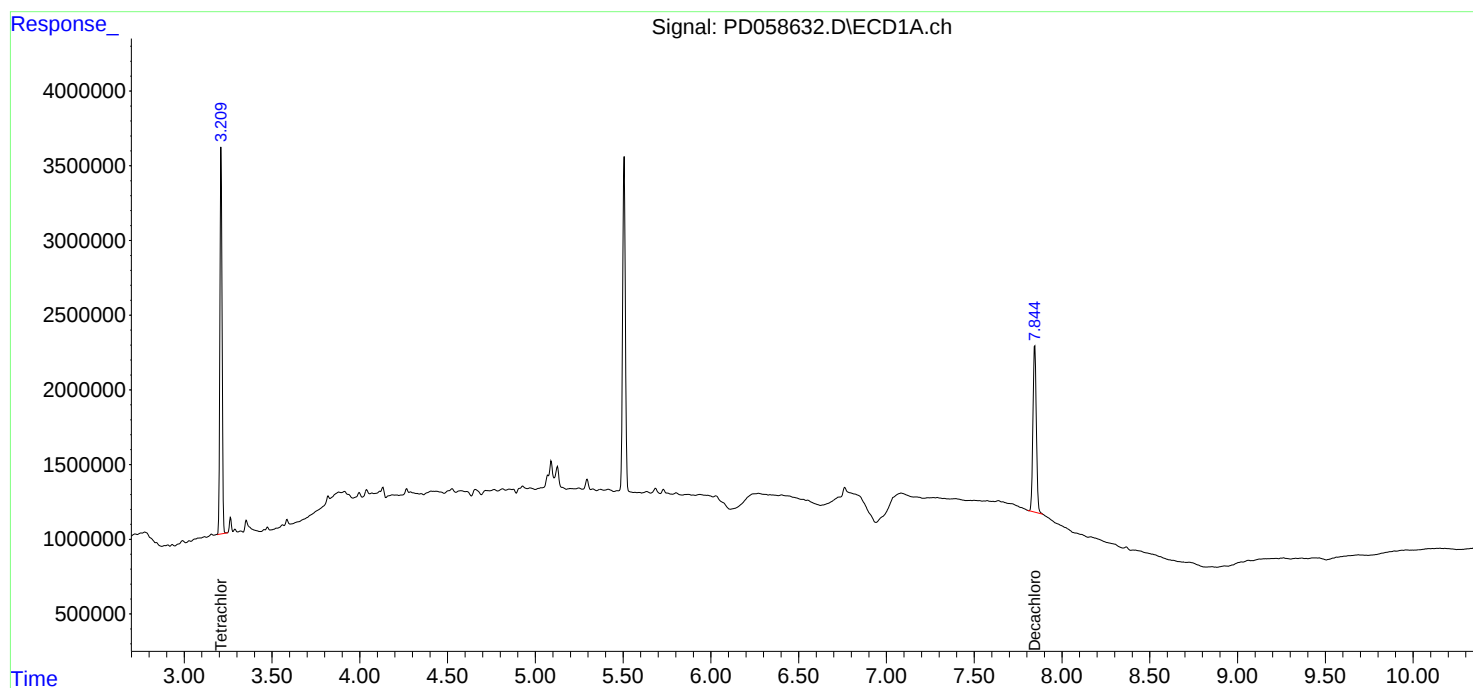


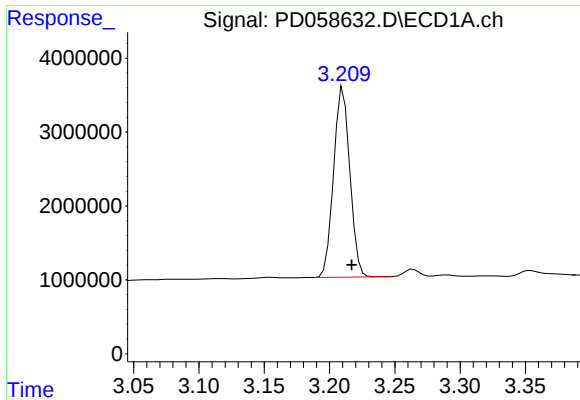

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: -0.006 min
Response: 22280694
Conc: 12.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
1

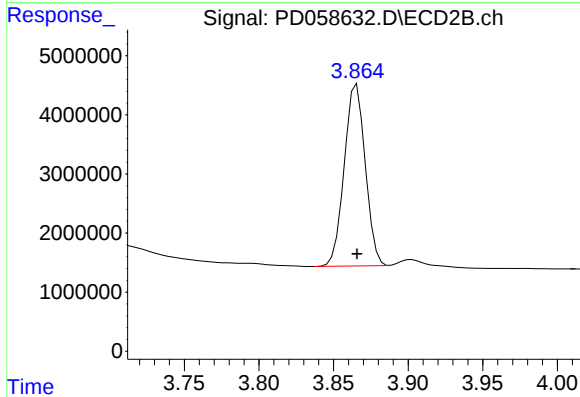


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 30169655
Conc: 12.21 ng/ml

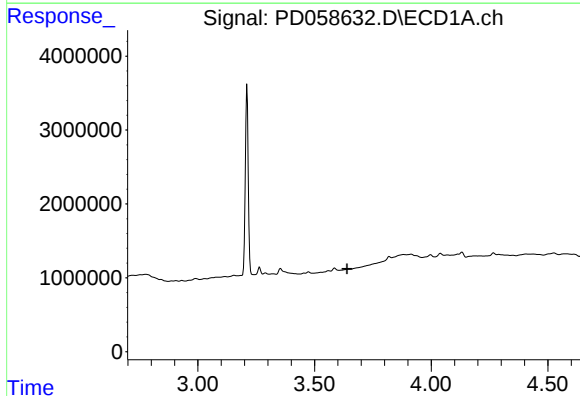


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.639 min
Response: 0
Conc: N.D.

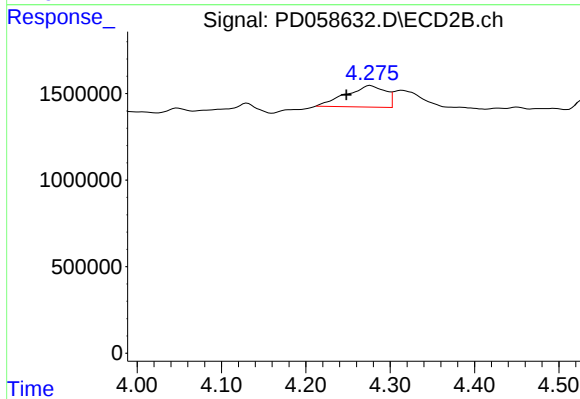

#2 alpha-BHC


R.T.: 4.277 min
Delta R.T.: 0.028 min
Response: 4045475
Conc: 1.07 ng/ml

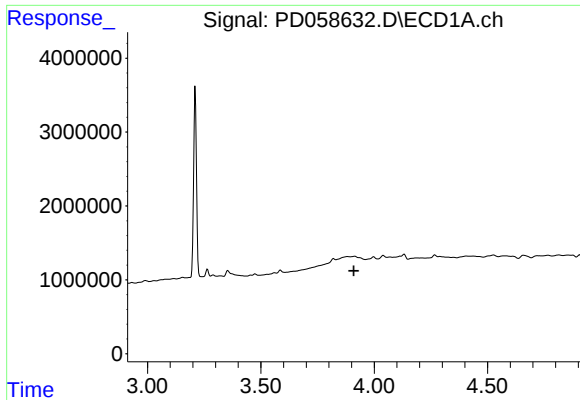

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
1

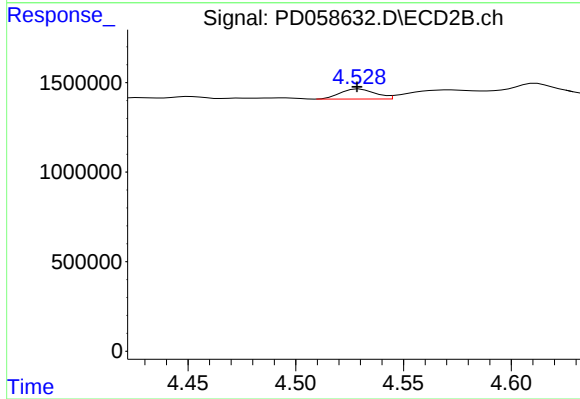


#3 gamma-BHC (Lindane)

R.T.: 4.530 min
Delta R.T.: 0.001 min
Response: 634685
Conc: 0.18 ng/ml

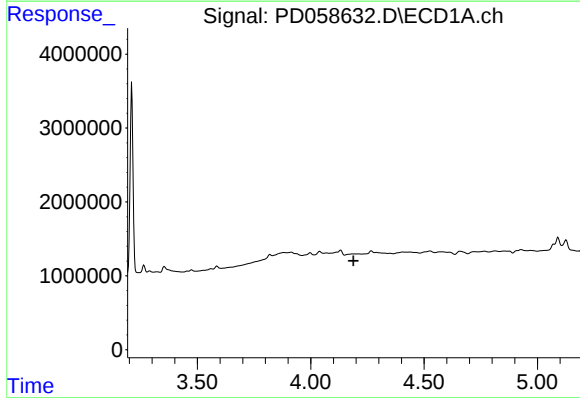


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.189 min
Response: 0
Conc: N.D.

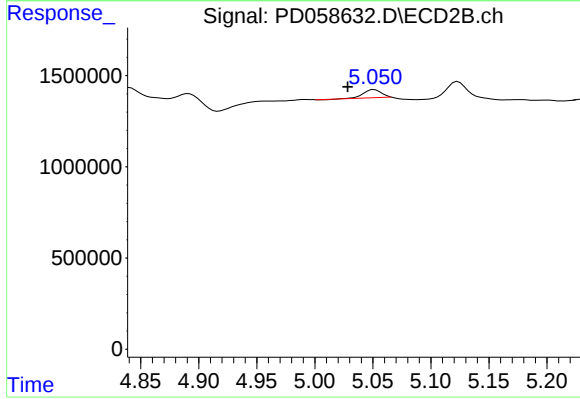

#4 Heptachlor


R.T.: 5.051 min
Delta R.T.: 0.023 min
Response: 485623
Conc: 0.15 ng/ml

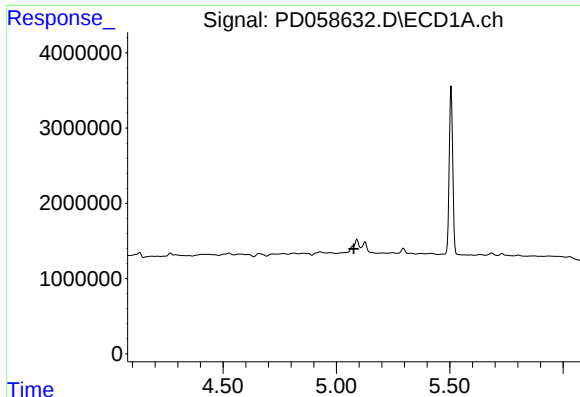

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
1

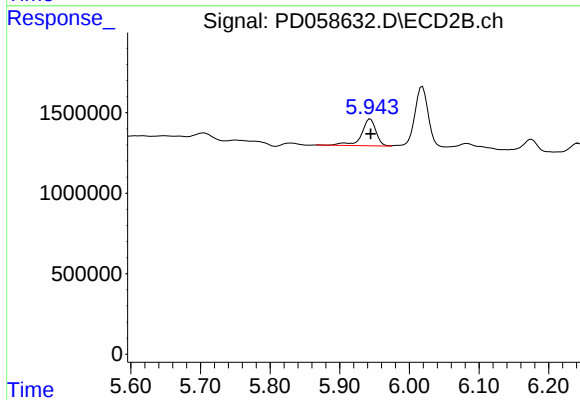


#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 2433593
Conc: 0.84 ng/ml

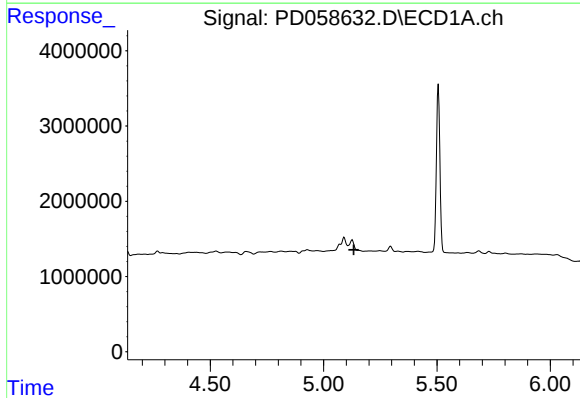


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

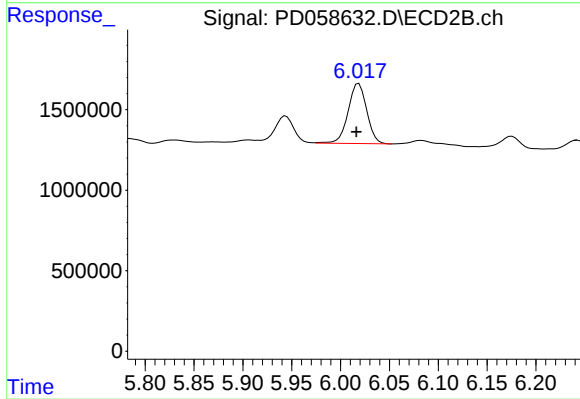

#11 alpha-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.003 min
Response: 4943470
Conc: 1.72 ng/ml

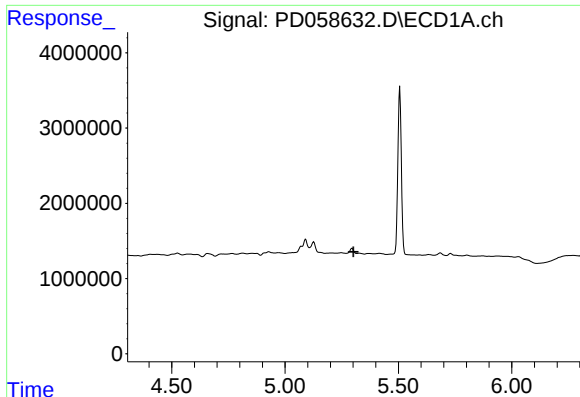

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
1

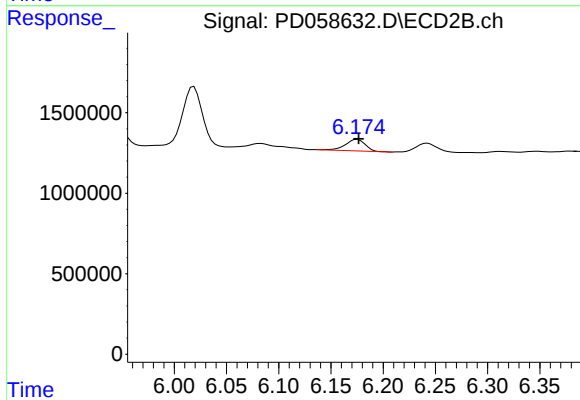


#12 4,4'-DDE

R.T.: 6.175 min
Delta R.T.: -0.001 min
Response: 952453
Conc: 0.35 ng/ml

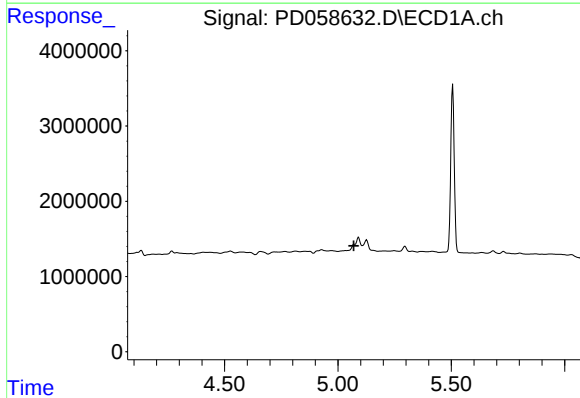


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

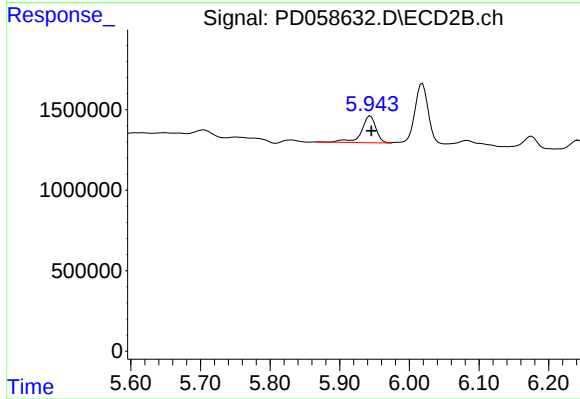

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: -0.001 min
Response: 2433593
Conc: 6.54 ng/ml

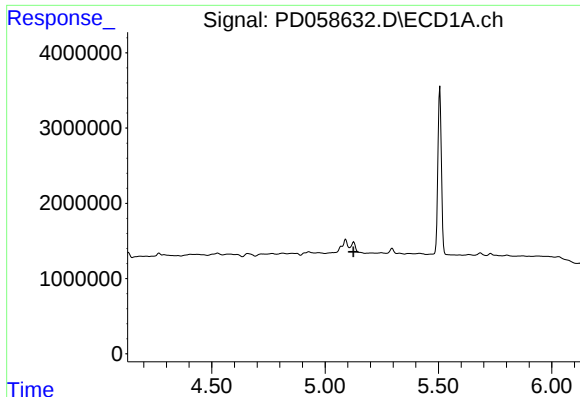

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
1

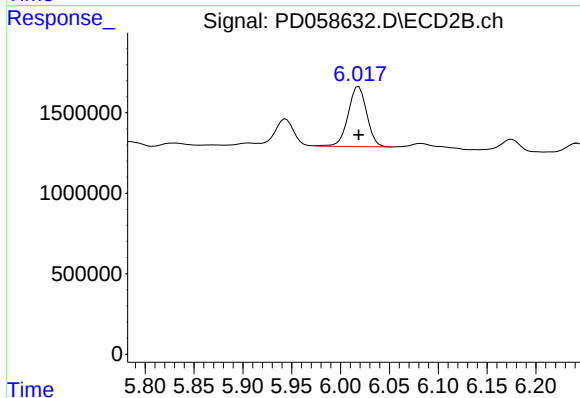


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 4943470
Conc: 11.36 ng/ml

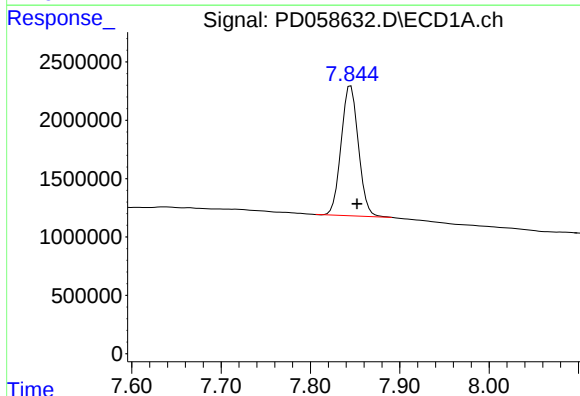

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: -0.007 min
Response: 14914048
Conc: 8.26 ng/ml

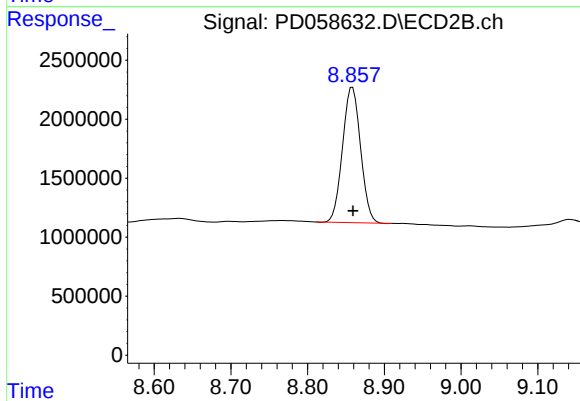

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 18786221
Conc: 8.62 ng/ml