

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 14:06
 Operator : AJ\MA
 Sample : L3308-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:50:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	23563627	33497028	12.924	13.557
28)	SA Decachlor...	7.844	8.858	19611958	24450334	10.860	11.214
Target Compounds							
2)	A alpha-BHC	0.000	4.277f	0	3291267	N.D.	0.873 #
3)	MA gamma-BHC...	0.000	4.529	0	1909467	N.D.	0.552 #
4)	MA Heptachlor	0.000	5.051f	0	493876	N.D.	0.157 #
8)	B Heptachlo...	0.000	5.708	0	2012045	N.D.	0.691 #
10)	B gamma-Chl...	5.089	5.944	918777	2494593	0.413	0.857 #
11)	B alpha-Chl...	0.000	6.018	0	5581601	N.D.	1.941 #
12)	B 4,4'-DDE	0.000	6.175	0	978248	N.D.	0.356 #
25)	Chlordane-3	5.089f	5.944	918777	2494593	4.489	6.707 #
26)	Chlordane-4	0.000	6.018	0	5581601	N.D.	12.831 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 14:06
Operator : AJ\MA
Sample : L3308-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:50:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

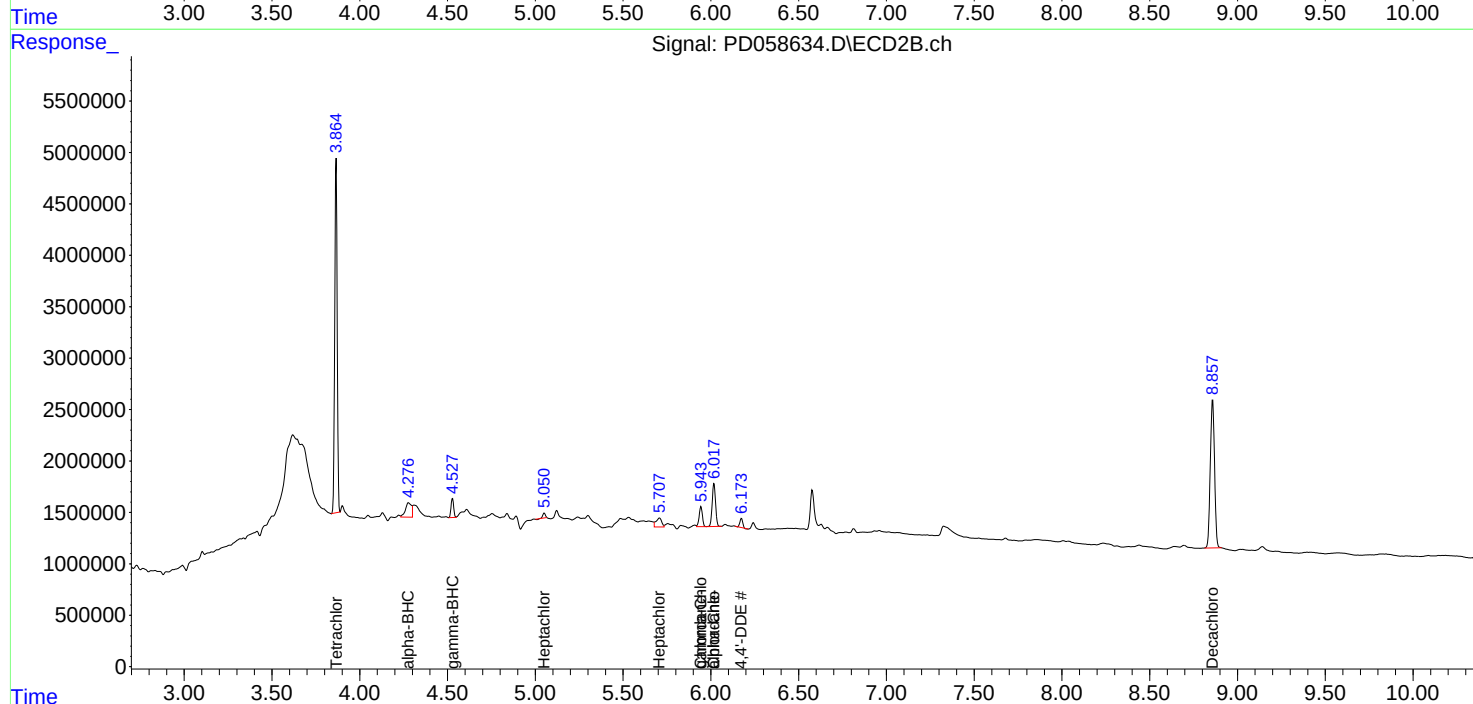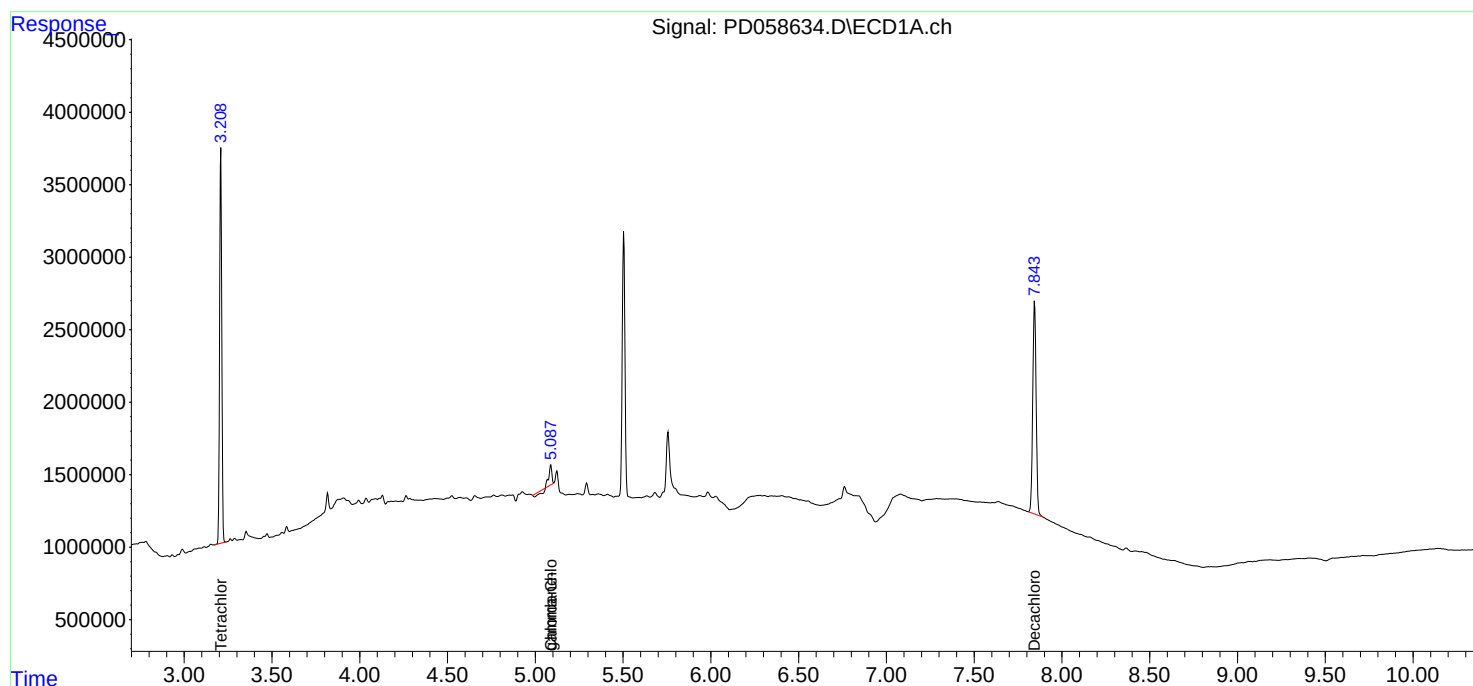


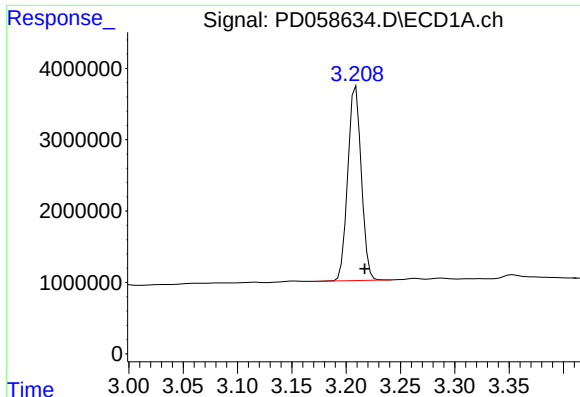

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 23563627
Conc: 12.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
3

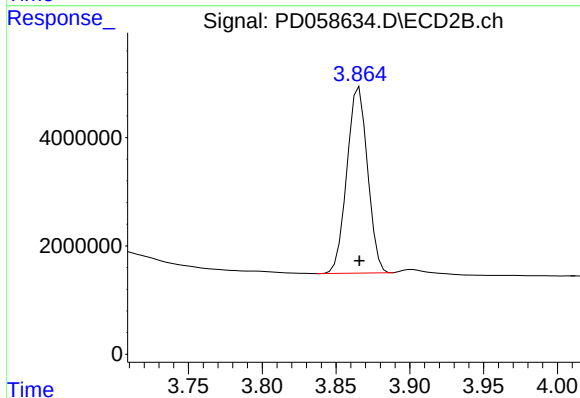


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 33497028
Conc: 13.56 ng/ml

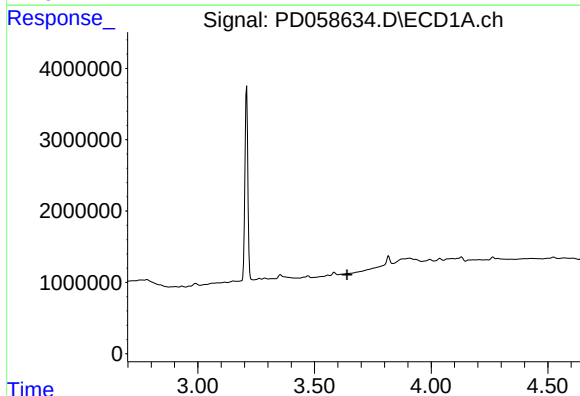


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.639 min
Response: 0
Conc: N.D.

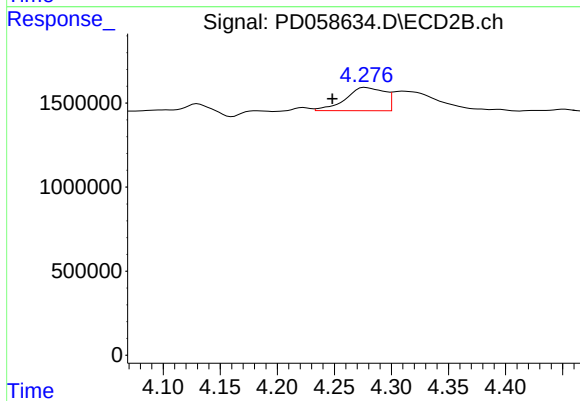

#2 alpha-BHC


R.T.: 4.277 min
Delta R.T.: 0.029 min
Response: 3291267
Conc: 0.87 ng/ml

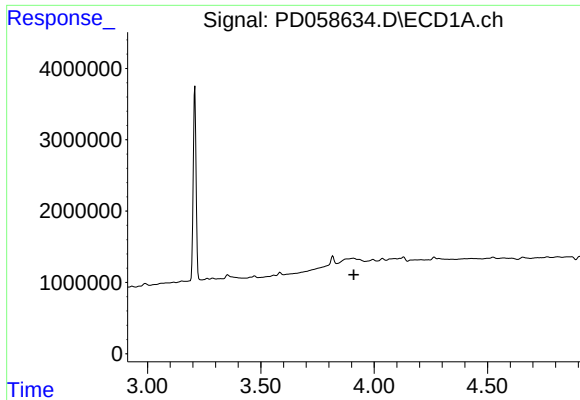

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
3

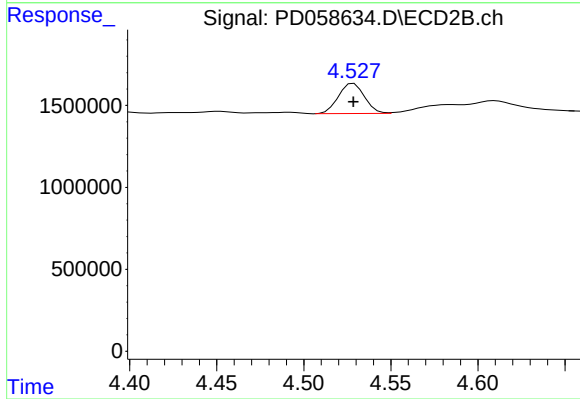


#3 gamma-BHC (Lindane)

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 1909467
Conc: 0.55 ng/ml

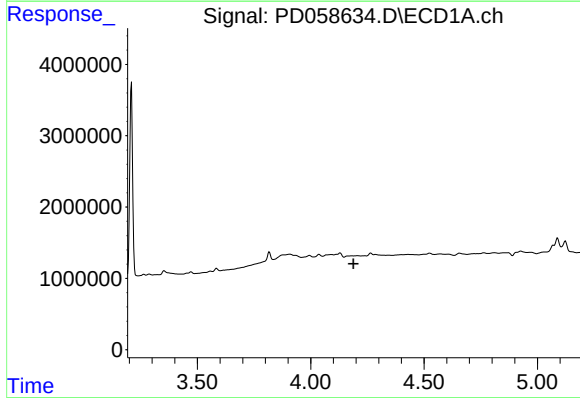


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.189 min
Response: 0
Conc: N.D.

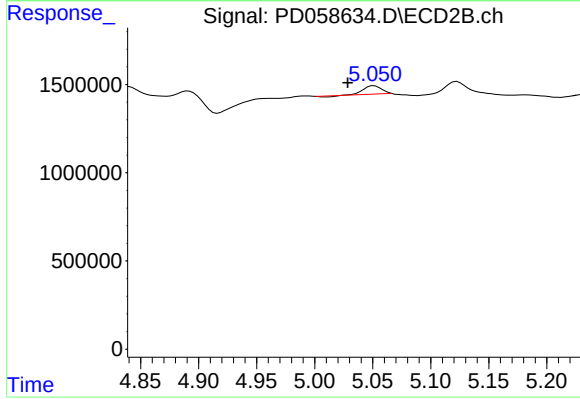

#4 Heptachlor


R.T.: 5.051 min
Delta R.T.: 0.023 min
Response: 493876
Conc: 0.16 ng/ml

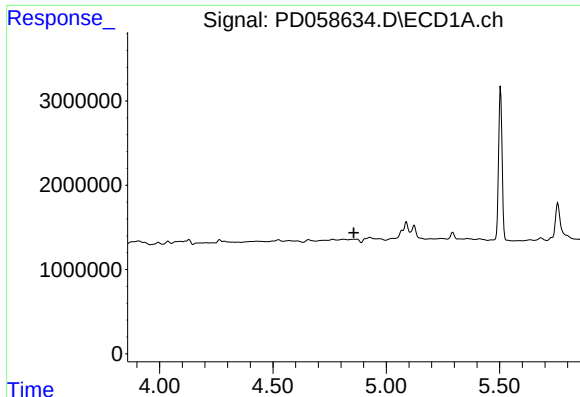

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
3

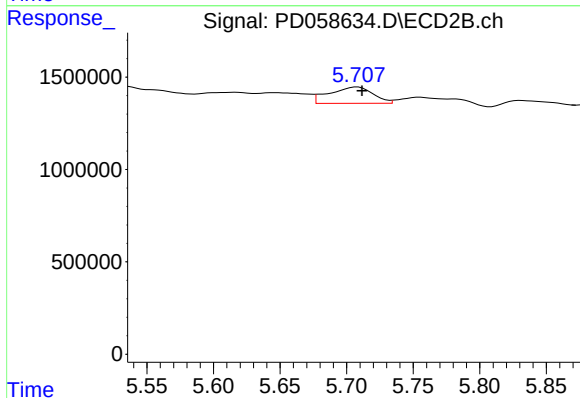


#8 Heptachlor epoxide

R.T.: 5.708 min
Delta R.T.: -0.004 min
Response: 2012045
Conc: 0.69 ng/ml

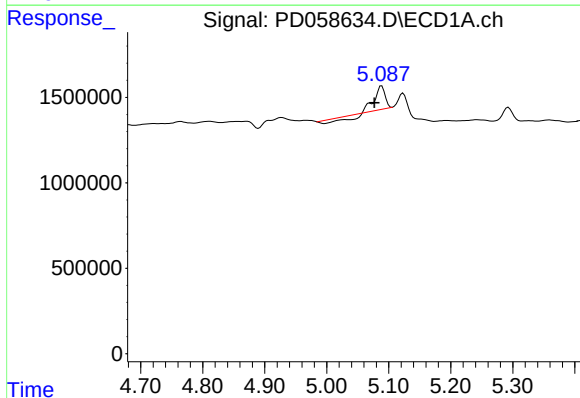


#10 gamma-Chlordane

R.T.: 5.089 min
Delta R.T.: 0.012 min
Response: 918777
Conc: 0.41 ng/ml

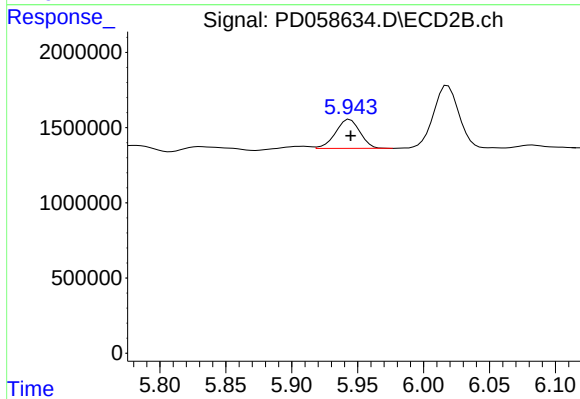

#10 gamma-Chlordane


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 2494593
Conc: 0.86 ng/ml

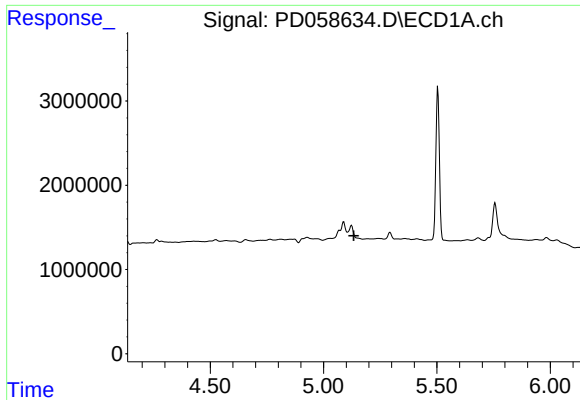

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
3

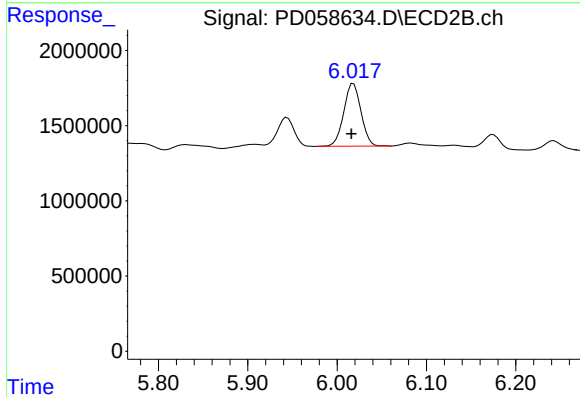


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.002 min
Response: 5581601
Conc: 1.94 ng/ml

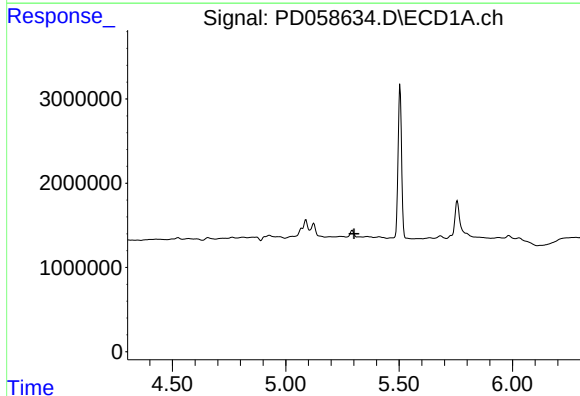


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

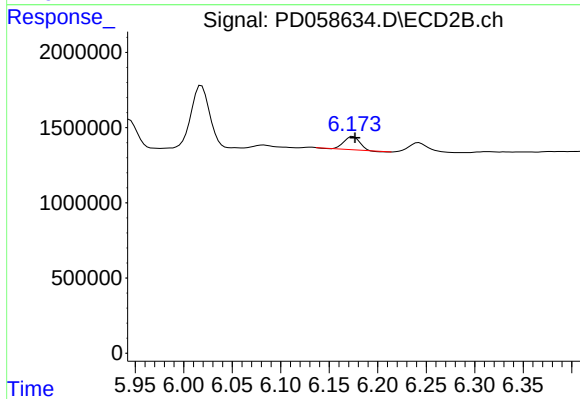

#12 4,4'-DDE


R.T.: 6.175 min
Delta R.T.: -0.002 min
Response: 978248
Conc: 0.36 ng/ml

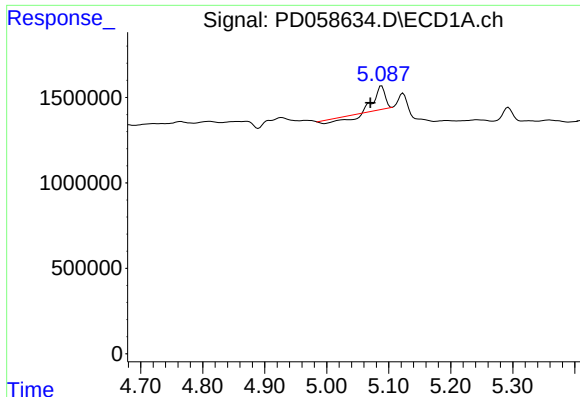

#25 Chlordane-3


R.T.: 5.089 min
Delta R.T.: 0.018 min
Response: 918777
Conc: 4.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
3

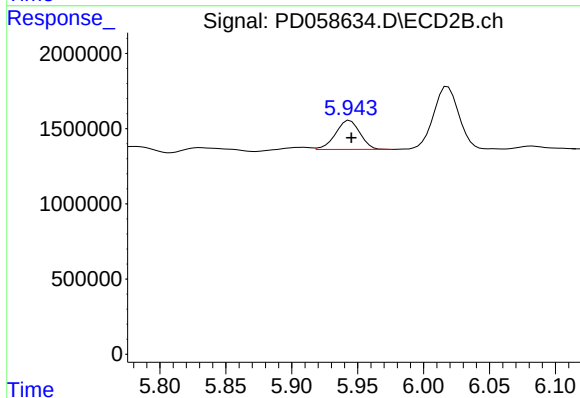


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: -0.001 min
Response: 2494593
Conc: 6.71 ng/ml

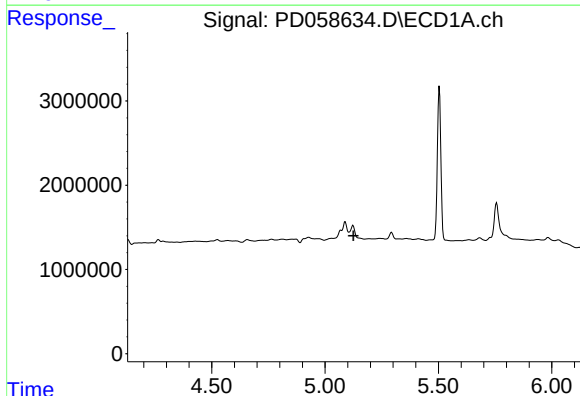


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.126 min
Response: 0
Conc: N.D.

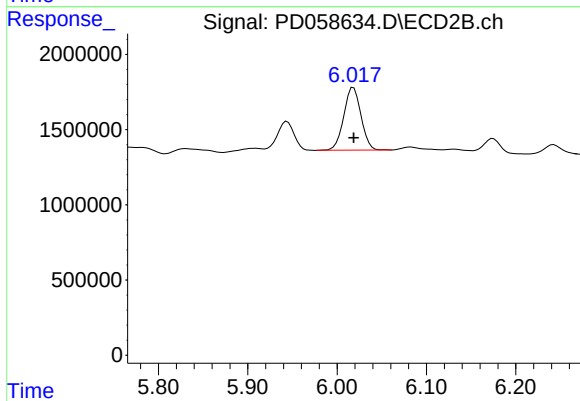

#26 Chlordane-4


R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 5581601
Conc: 12.83 ng/ml

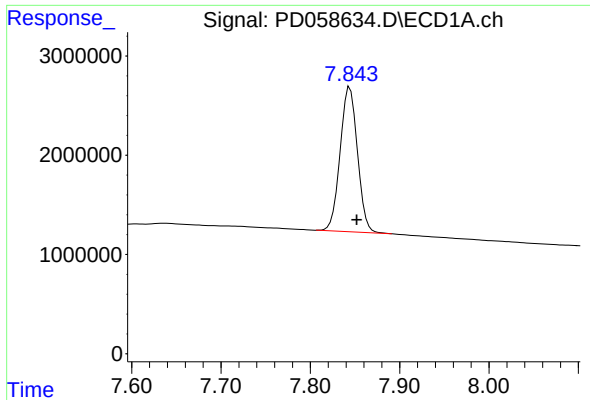

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 19611958
Conc: 10.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
3

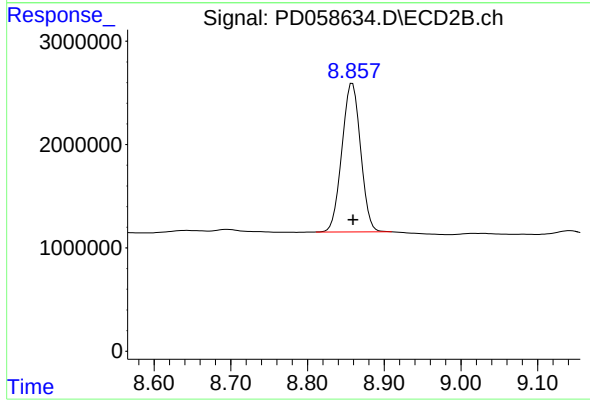

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 24450334
Conc: 11.21 ng/ml