

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 14:35
 Operator : AJ\MA
 Sample : L3308-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:50:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.865	23017706	32666144	12.624	13.221
28)	SA Decachlor...	7.844	8.858	18997916	23052800	10.520	10.573
Target Compounds							
2)	A alpha-BHC	0.000	4.278f	0	3394733	N.D.	0.900 #
4)	MA Heptachlor	0.000	5.051f	0	492305	N.D.	0.156 #
8)	B Heptachlo...	0.000	5.706	0	2950495	N.D.	1.014 #
10)	B gamma-Chl...	0.000	5.944	0	2292653	N.D.	0.788 #
11)	B alpha-Chl...	0.000	6.018	0	5270571	N.D.	1.833 #
12)	B 4,4'-DDE	0.000	6.174	0	1230952	N.D.	0.448 #
25)	Chlordane-3	0.000	5.944	0	2292653	N.D.	6.164 #
26)	Chlordane-4	0.000	6.018	0	5270571	N.D.	12.116 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 14:35
Operator : AJ\MA
Sample : L3308-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:50:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

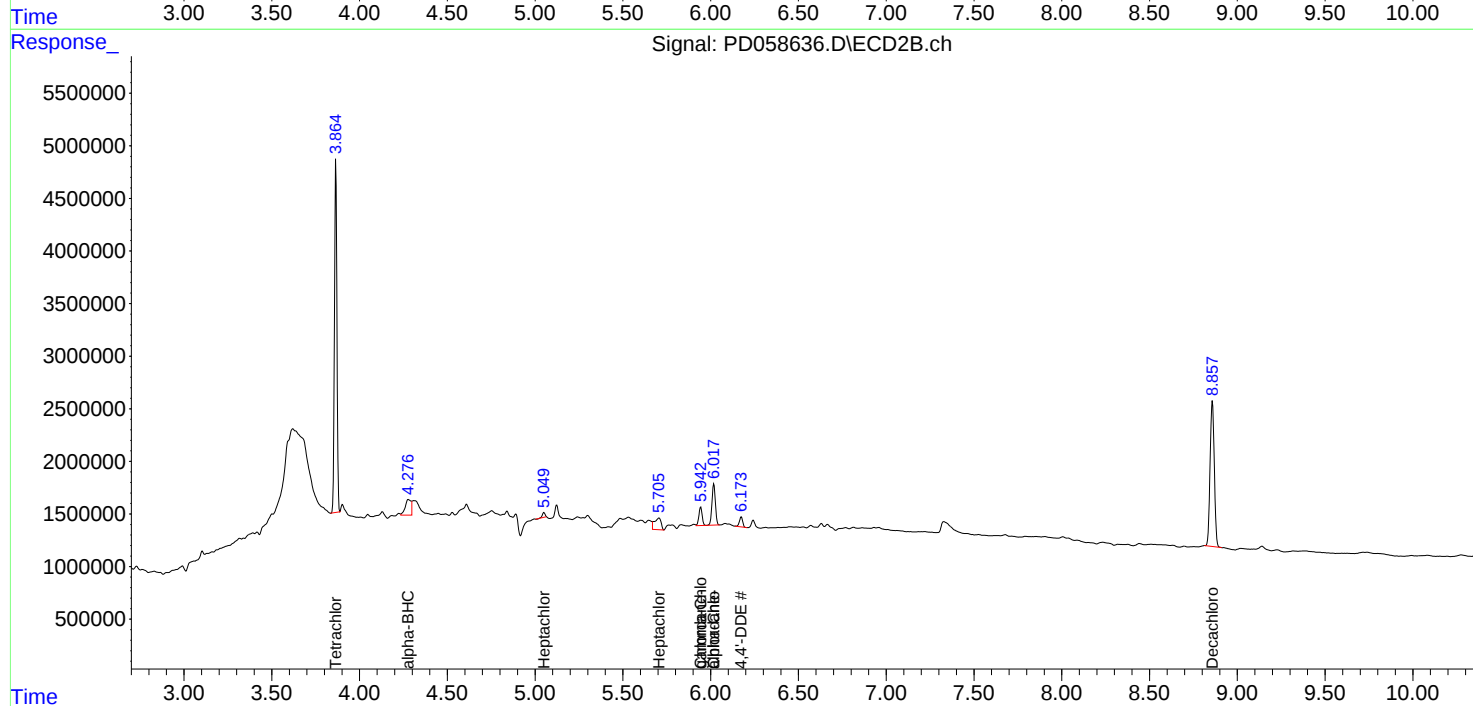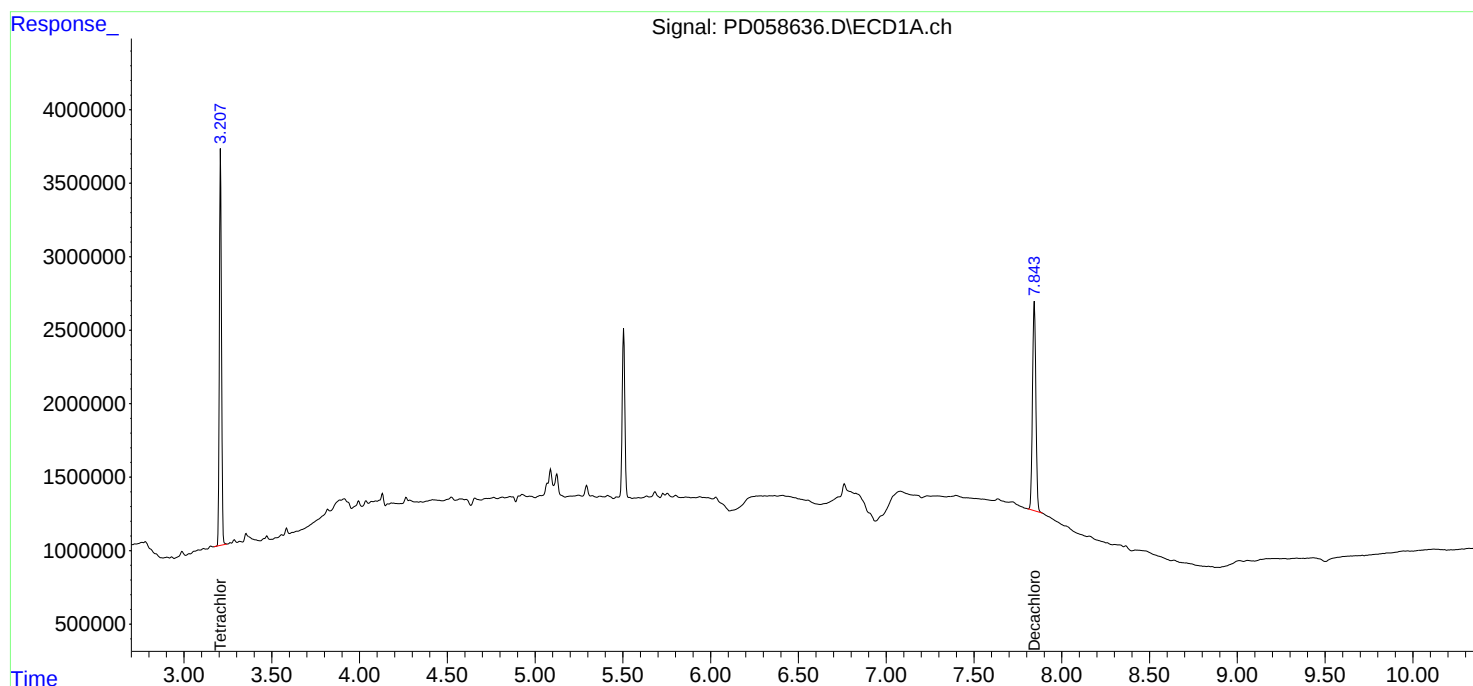


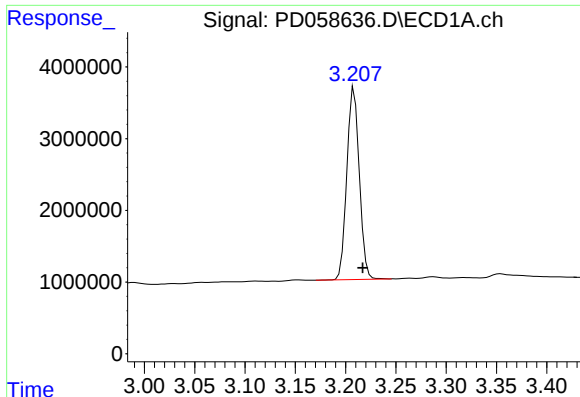

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 23017706
Conc: 12.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

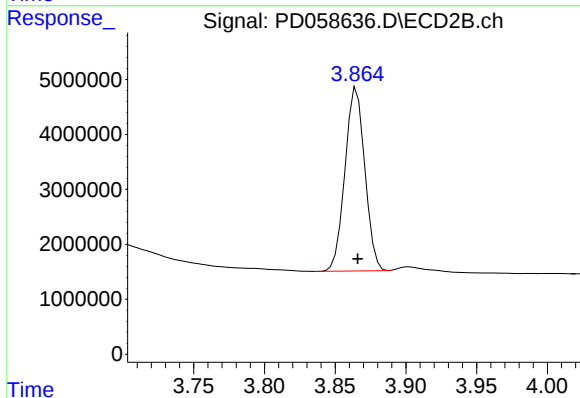


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 32666144
Conc: 13.22 ng/ml

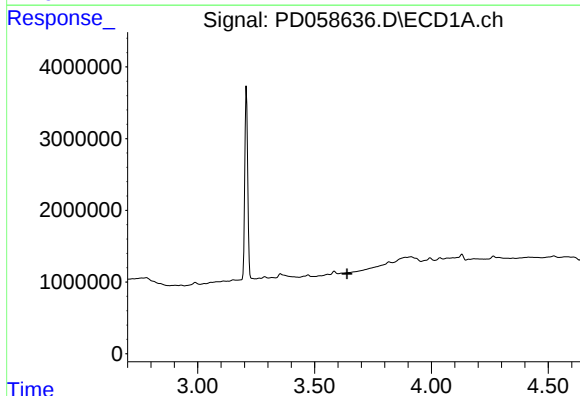


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.639 min
Response: 0
Conc: N.D.

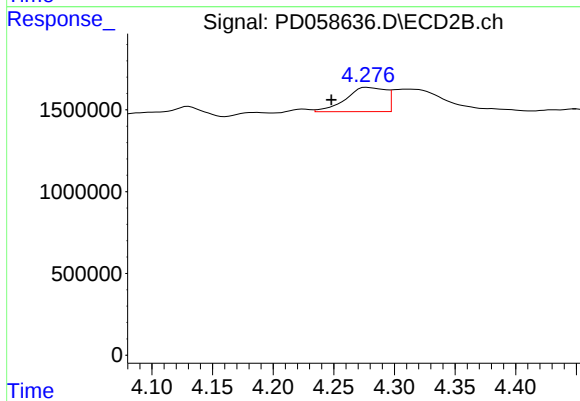

#2 alpha-BHC


R.T.: 4.278 min
Delta R.T.: 0.029 min
Response: 3394733
Conc: 0.90 ng/ml

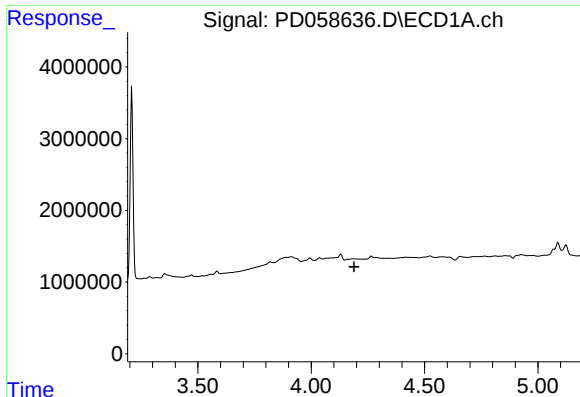

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

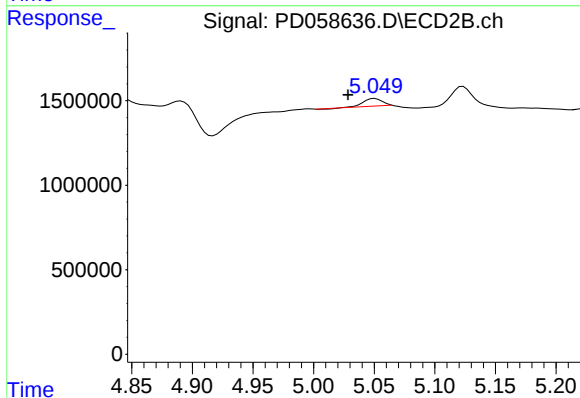


#4 Heptachlor

R.T.: 5.051 min
Delta R.T.: 0.022 min
Response: 492305
Conc: 0.16 ng/ml

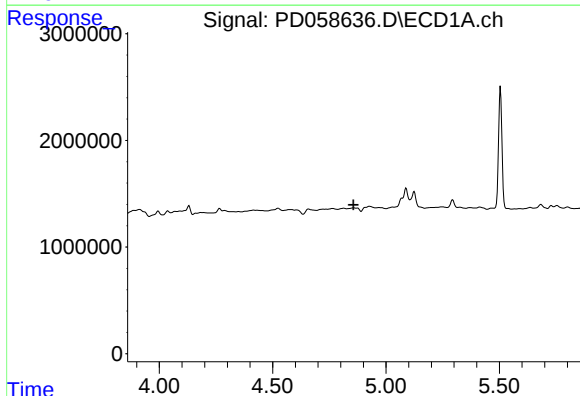


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.857 min
Response: 0
Conc: N.D.

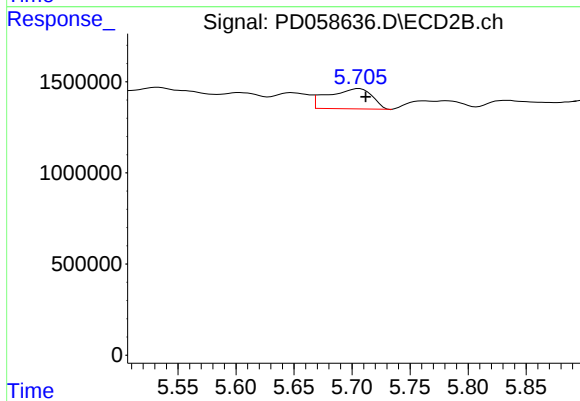

#8 Heptachlor epoxide


R.T.: 5.706 min
Delta R.T.: -0.006 min
Response: 2950495
Conc: 1.01 ng/ml

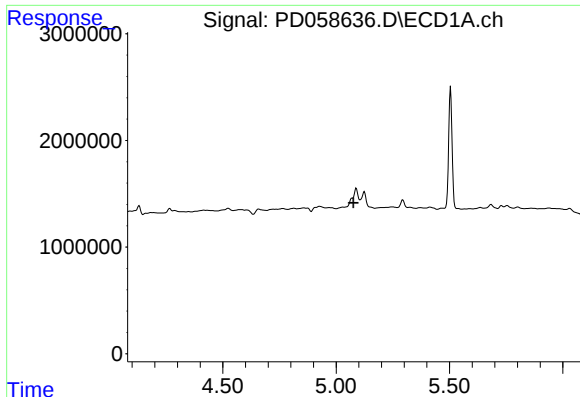

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

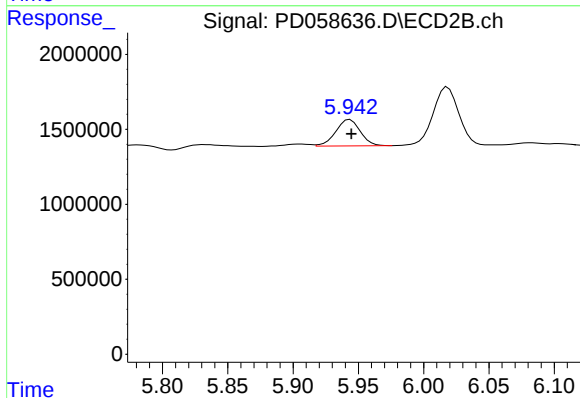


#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.001 min
Response: 2292653
Conc: 0.79 ng/ml

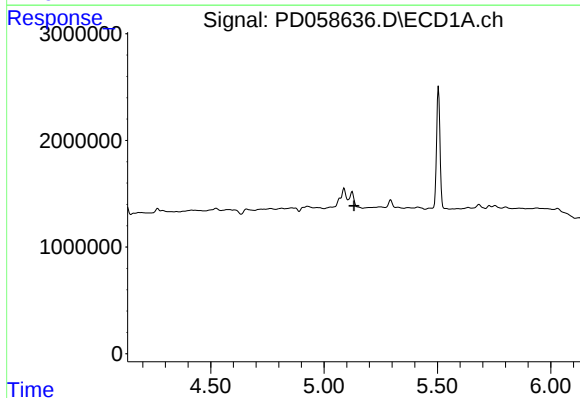


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

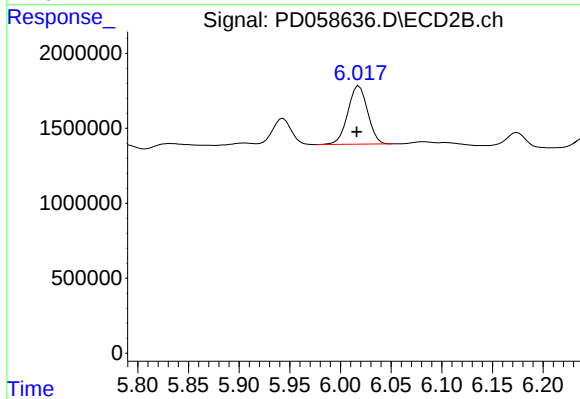

#11 alpha-Chlordane


R.T.: 6.018 min
Delta R.T.: 0.002 min
Response: 5270571
Conc: 1.83 ng/ml

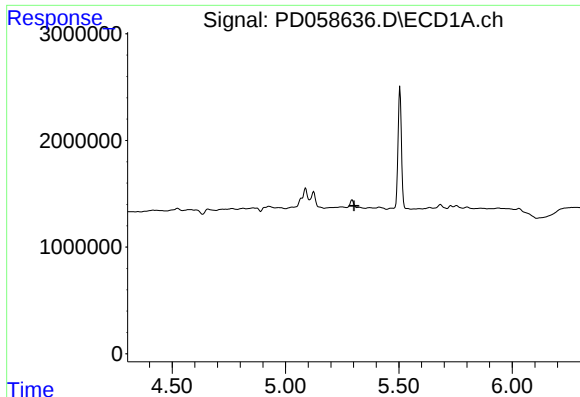

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

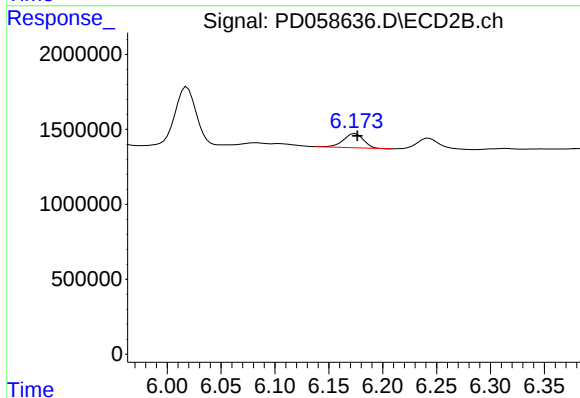


#12 4,4'-DDE

R.T.: 6.174 min
Delta R.T.: -0.002 min
Response: 1230952
Conc: 0.45 ng/ml

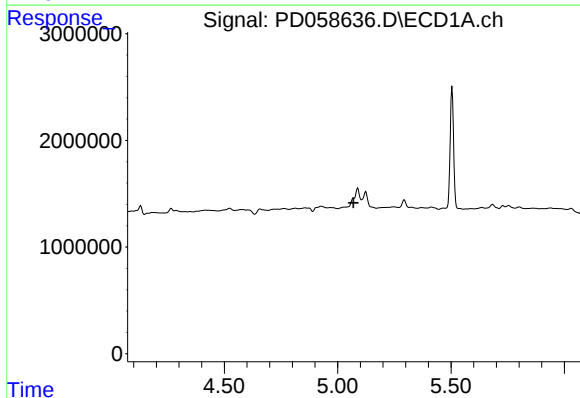


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

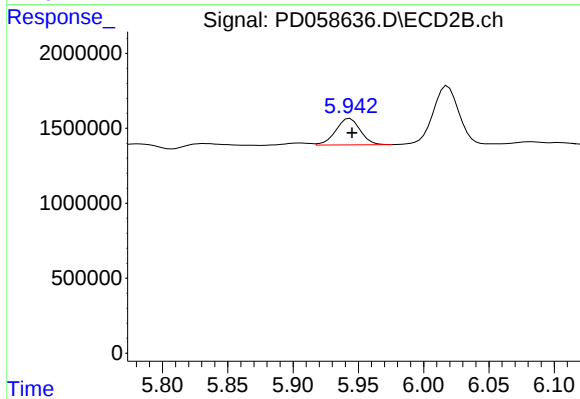

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: -0.002 min
Response: 2292653
Conc: 6.16 ng/ml

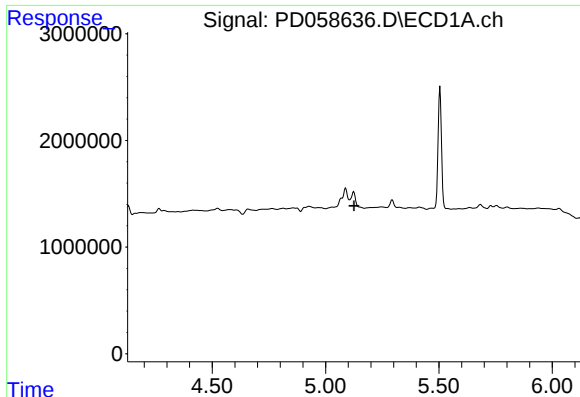

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

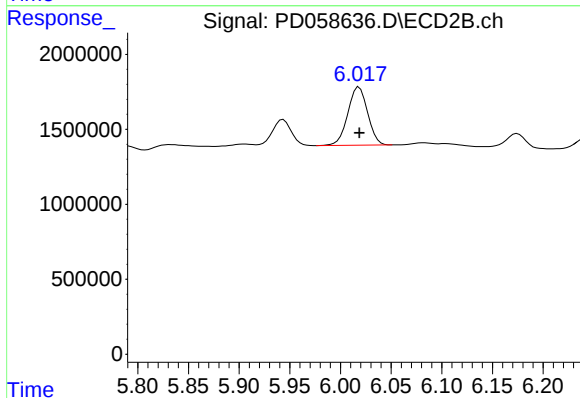


#26 Chlordane-4

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 5270571
Conc: 12.12 ng/ml

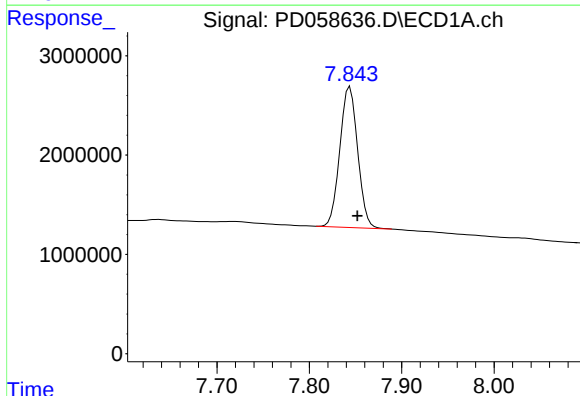

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 18997916
Conc: 10.52 ng/ml

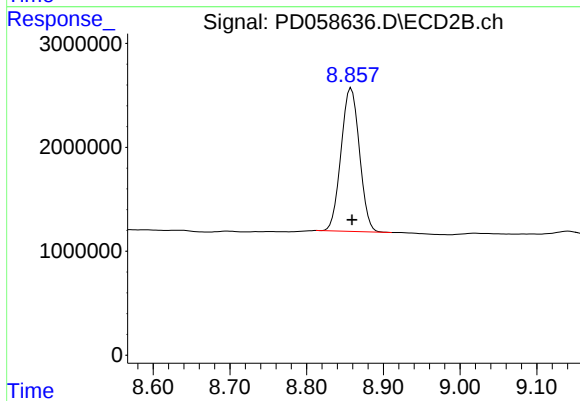

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: -0.001 min
Response: 23052800
Conc: 10.57 ng/ml