

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 15:04
 Operator : AJ\MA
 Sample : L3308-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:51:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.865	20720864	29590456	11.364	11.976
28)	SA Decachlor...	7.844	8.858	15764358	19416475	8.730	8.905
Target Compounds							
3)	MA gamma-BHC...	0.000	4.528	0	1360081	N.D.	0.393 #
8)	B Heptachlo...	0.000	5.708	0	1927993	N.D.	0.662 #
10)	B gamma-Chl...	0.000	5.943	0	1735499	N.D.	0.596 #
11)	B alpha-Chl...	0.000	6.018	0	3980317	N.D.	1.384 #
12)	B 4,4'-DDE	0.000	6.174	0	962989	N.D.	0.350 #
25)	Chlordane-3	0.000	5.943	0	1735499	N.D.	4.666 #
26)	Chlordane-4	0.000	6.018	0	3980317	N.D.	9.150 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 15:04
Operator : AJ\MA
Sample : L3308-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:51:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

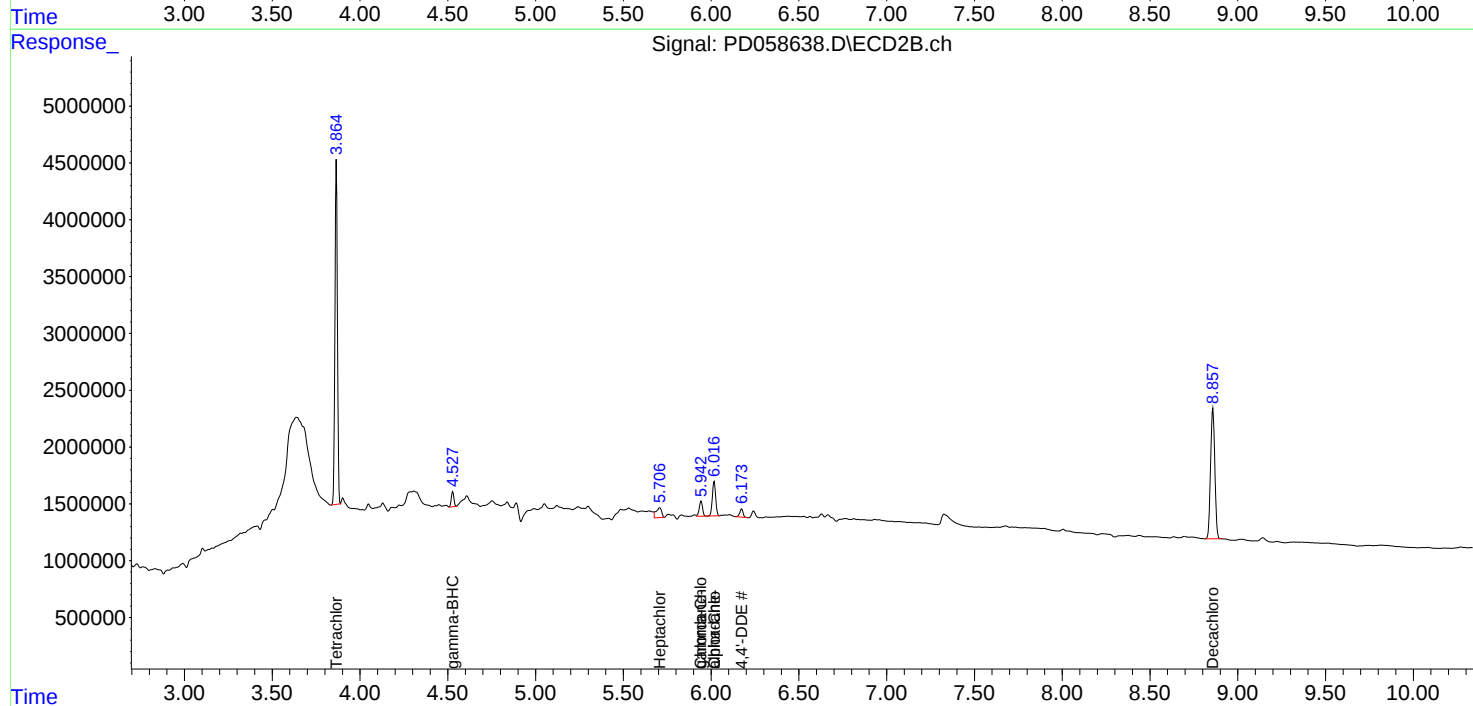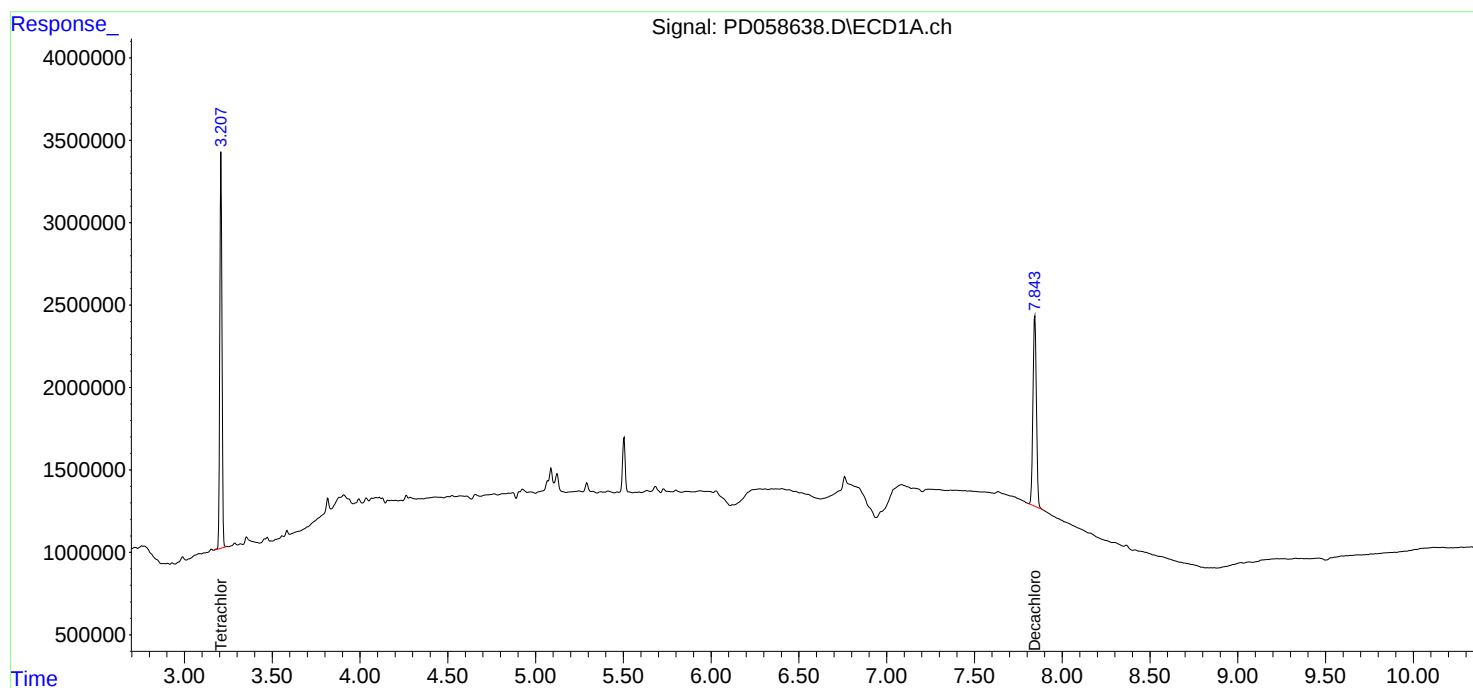


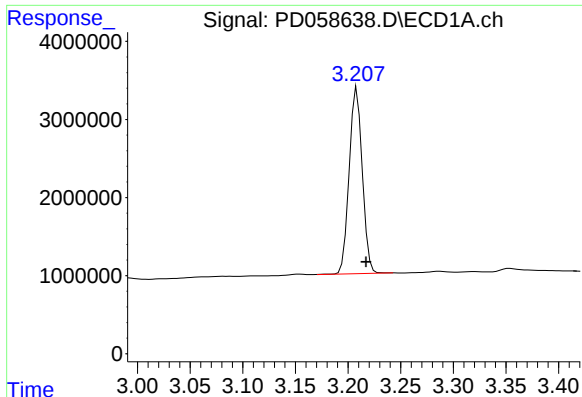

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 20720864
Conc: 11.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
7

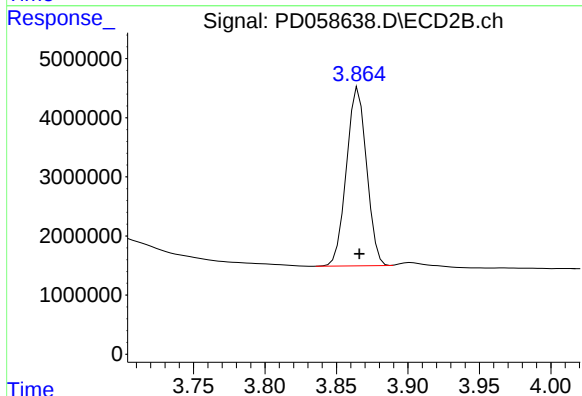


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 29590456
Conc: 11.98 ng/ml

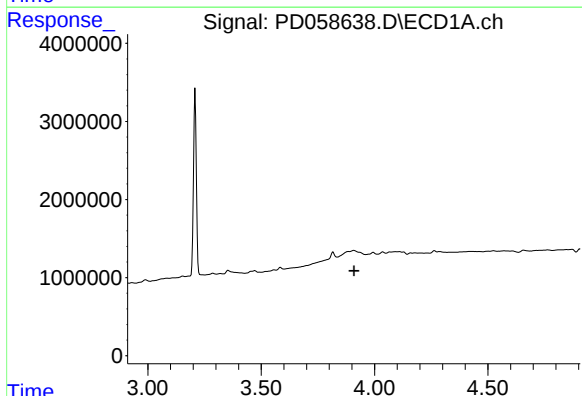


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

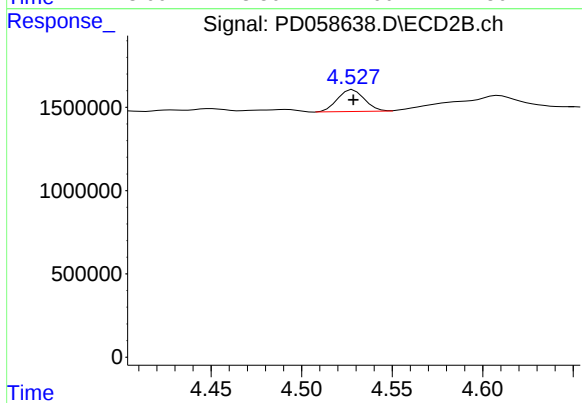

#3 gamma-BHC (Lindane)


R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 1360081
Conc: 0.39 ng/ml

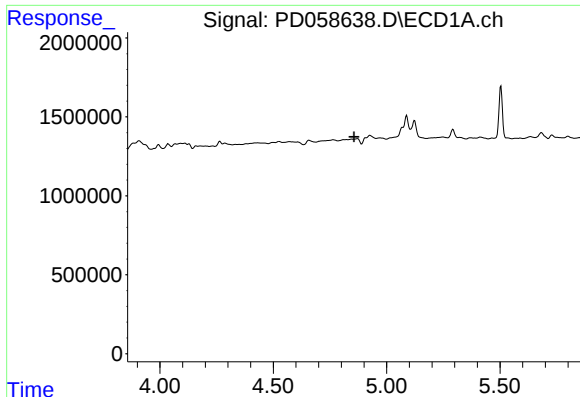

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
7

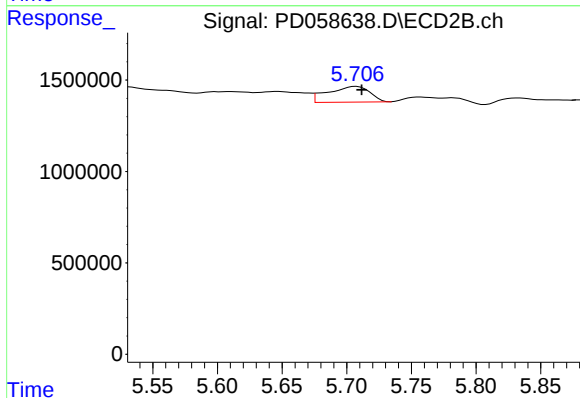


#8 Heptachlor epoxide

R.T.: 5.708 min
Delta R.T.: -0.004 min
Response: 1927993
Conc: 0.66 ng/ml

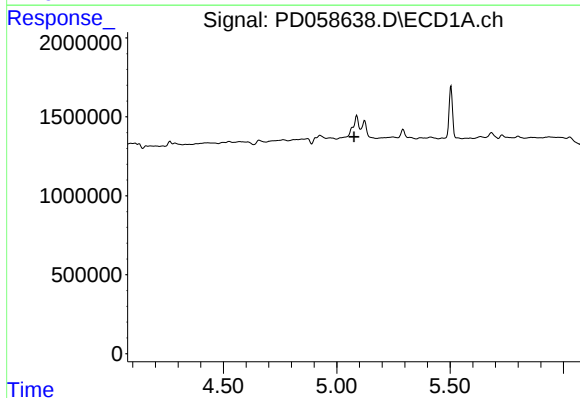


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

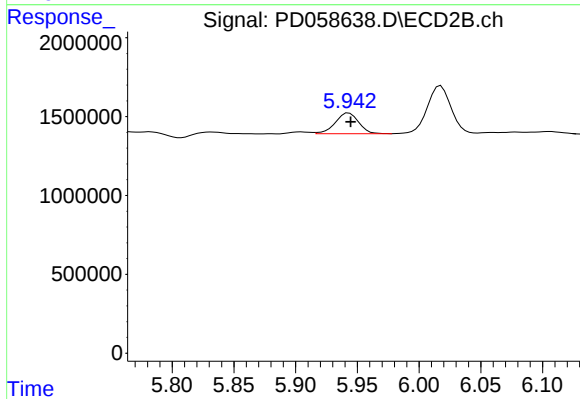

#10 gamma-Chlordane


R.T.: 5.943 min
Delta R.T.: -0.002 min
Response: 1735499
Conc: 0.60 ng/ml

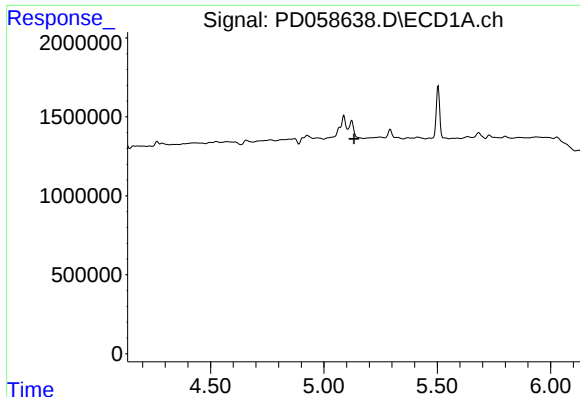

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
7

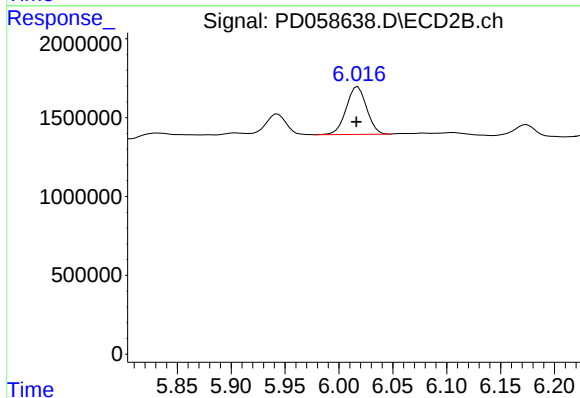


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.001 min
Response: 3980317
Conc: 1.38 ng/ml

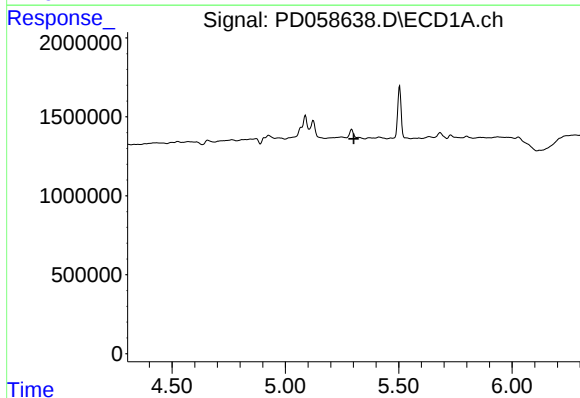


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

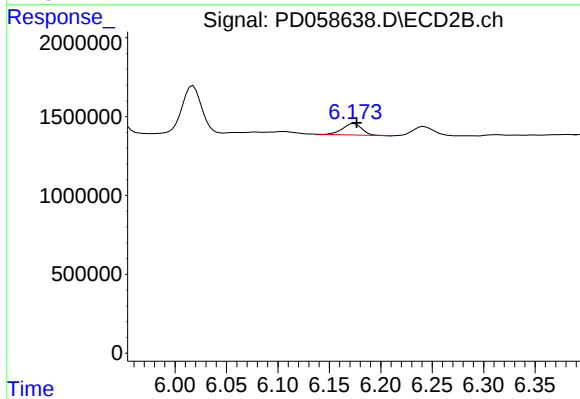

#12 4,4'-DDE


R.T.: 6.174 min
Delta R.T.: -0.003 min
Response: 962989
Conc: 0.35 ng/ml

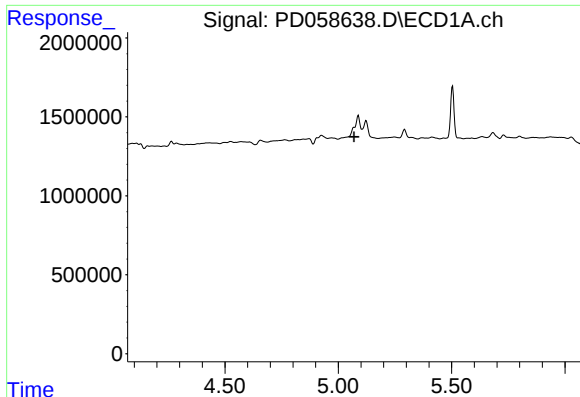

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
7

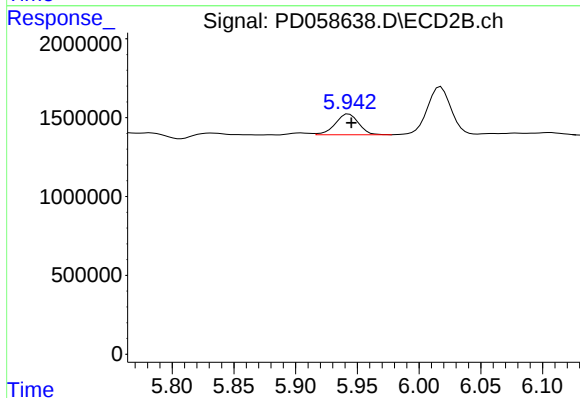


#25 Chlordane-3

R.T.: 5.943 min
Delta R.T.: -0.002 min
Response: 1735499
Conc: 4.67 ng/ml

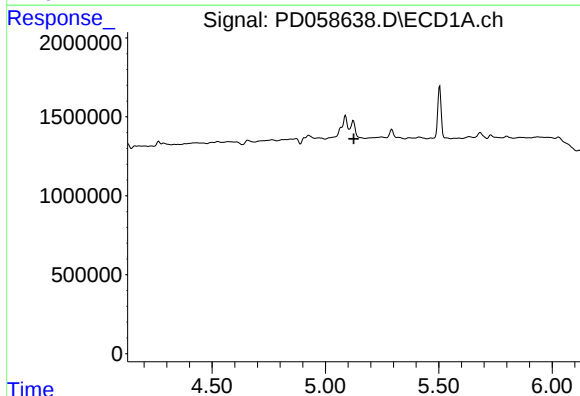


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

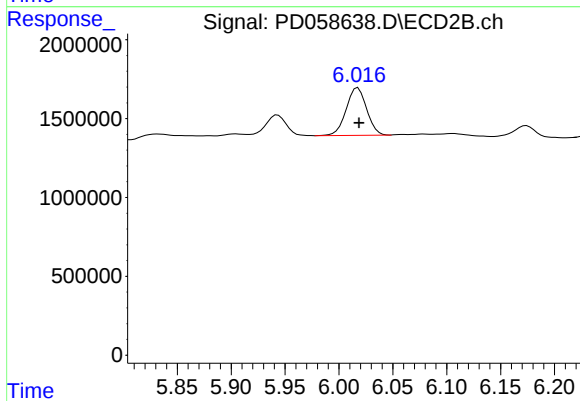

#26 Chlordane-4


R.T.: 6.018 min
Delta R.T.: -0.001 min
Response: 3980317
Conc: 9.15 ng/ml

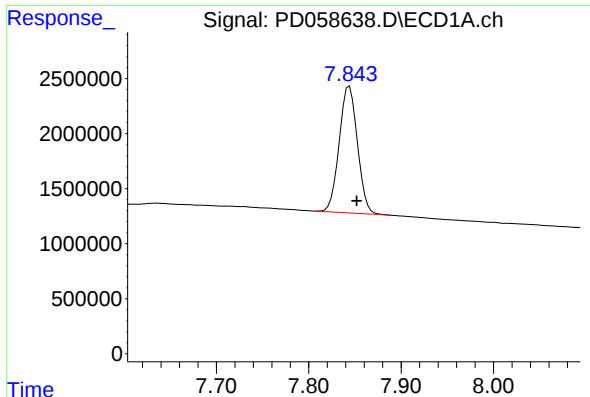

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 15764358
Conc: 8.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
7

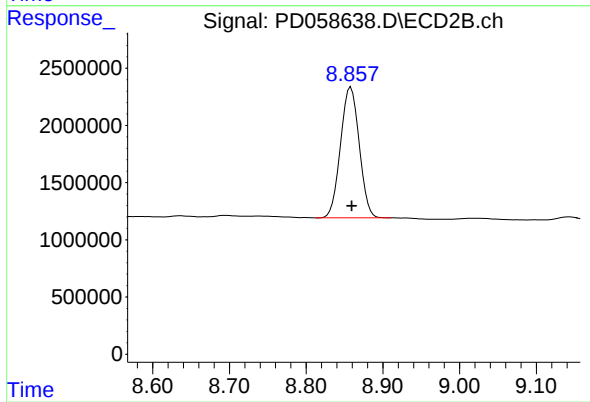

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 19416475
Conc: 8.91 ng/ml