

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 14:06
 Operator : AJ\MA
 Sample : L3308-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 3

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:42:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:50:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.866	23563627	33497028	12.924	13.557
28) SA Decachlor...	7.844	8.858	19611958	24450334	10.860	11.214
Target Compounds						
10) B gamma-Chl...	5.068	5.944	1194329	2494593	0.536m	0.857 #
11) B alpha-Chl...	5.122	6.018	2035346	5581601	0.919m	1.941 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 14:06
Operator : AJ\MA
Sample : L3308-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
3


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:50:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

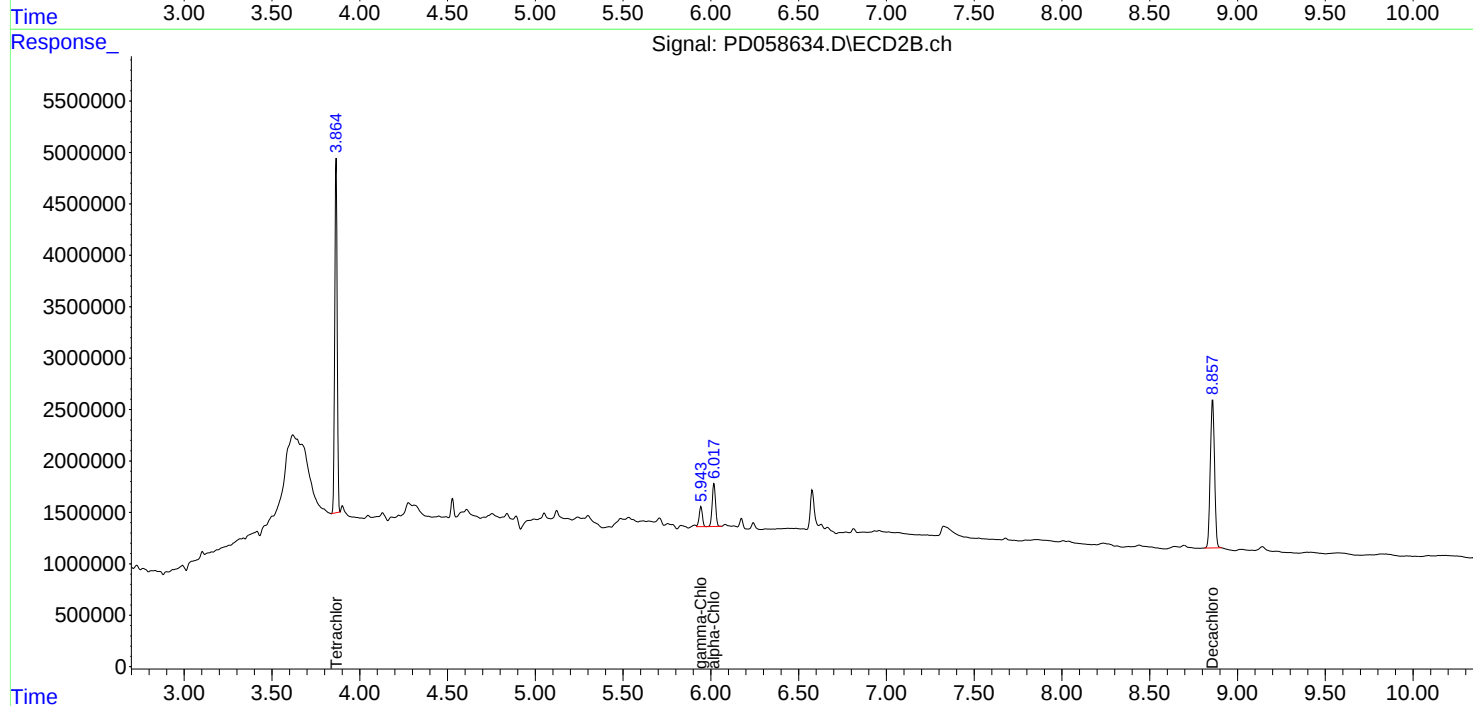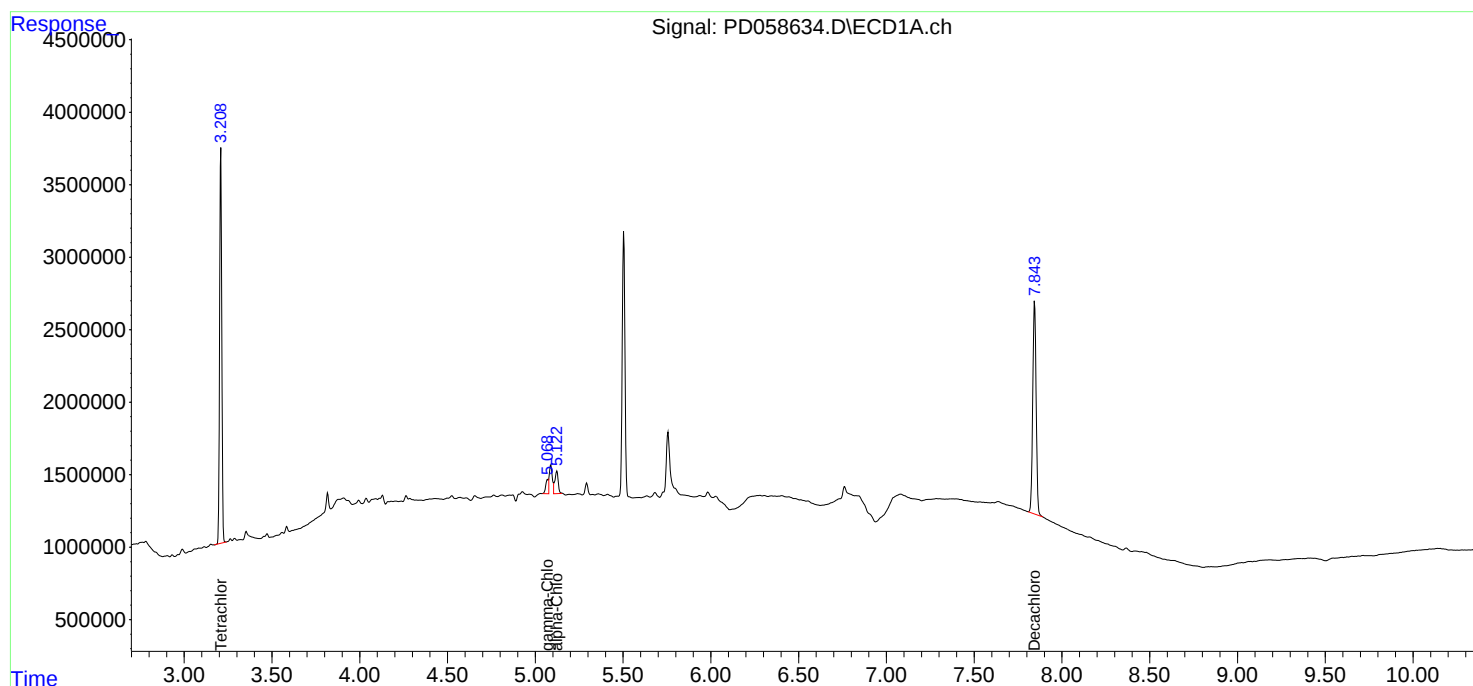

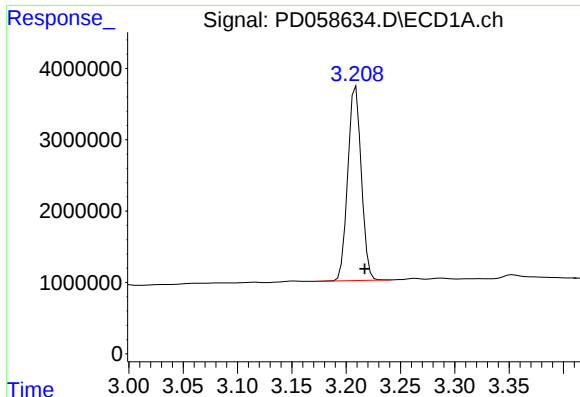


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 23563627
Conc: 12.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
3


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:16 AM

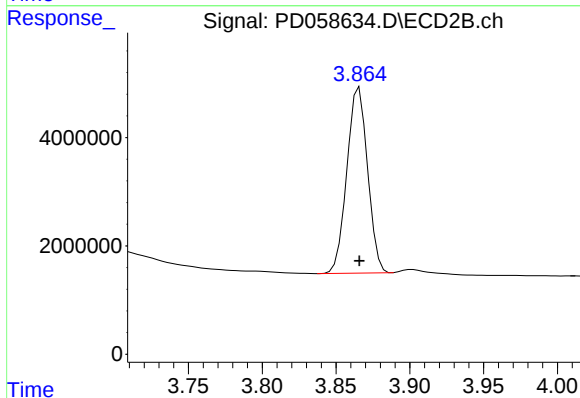


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 33497028
Conc: 13.56 ng/ml

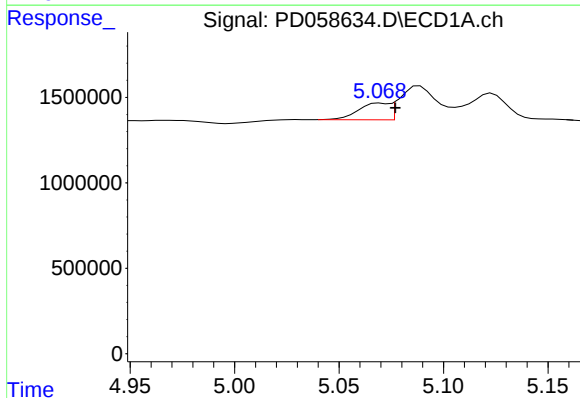


#10 gamma-Chlordane

R.T.: 5.068 min
Delta R.T.: -0.009 min
Response: 1194329
Conc: 0.54 ng/ml m

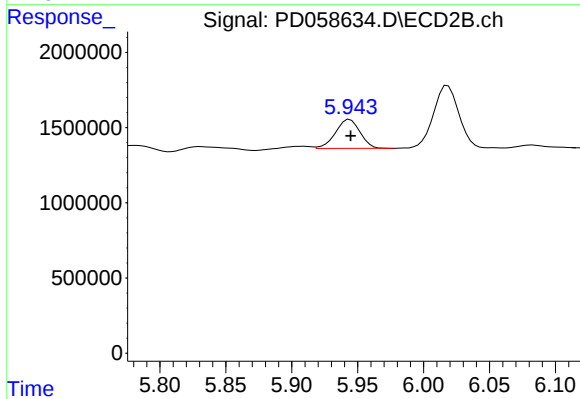

#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 2494593
Conc: 0.86 ng/ml

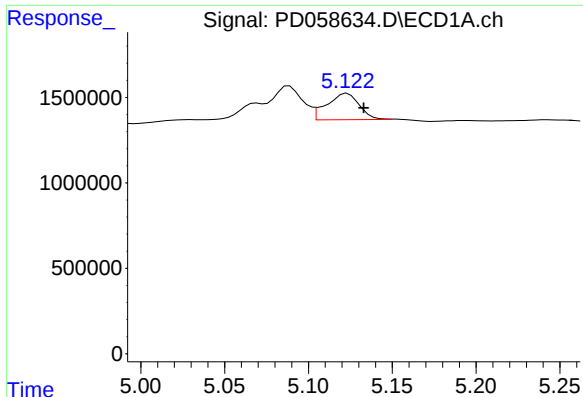


#11 alpha-Chlordane

R.T.: 5.122 min
Delta R.T.: -0.011 min
Response: 2035346
Conc: 0.92 ng/ml m

Instrument :
ECD_D
ClientSampleId :
3


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:16 AM

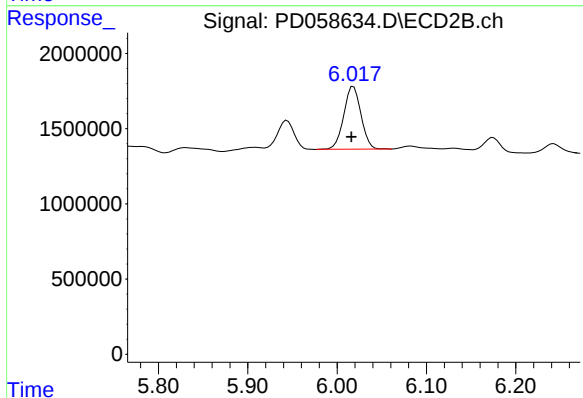


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.002 min
Response: 5581601
Conc: 1.94 ng/ml

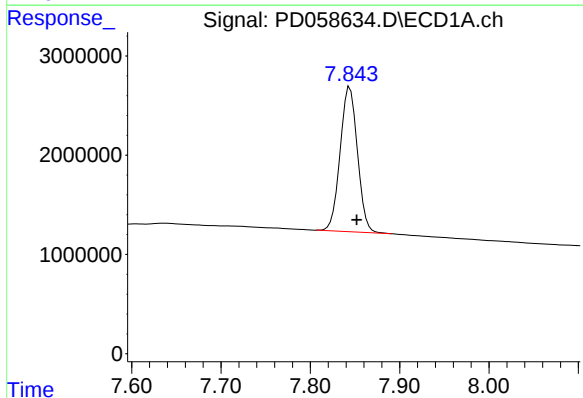

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 19611958
Conc: 10.86 ng/ml

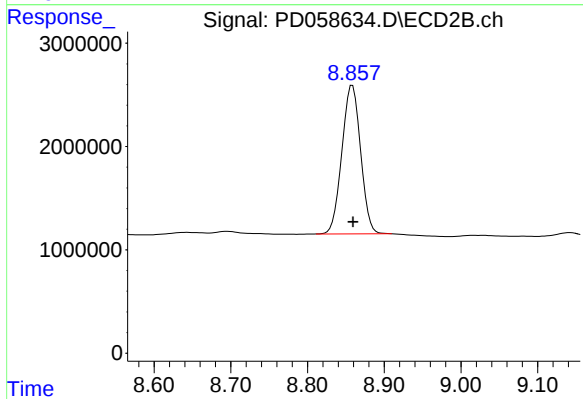

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 24450334
Conc: 11.21 ng/ml