

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 14:35
 Operator : AJ\MA
 Sample : L3308-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 5

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:42:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:50:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.865	23017706	32666144	12.624	13.221
28) SA Decachlor...	7.844	8.858	18997916	23052800	10.520	10.573
Target Compounds						
10) B gamma-Chl...	5.068	5.944	905485	2292653	0.407m	0.788 #
11) B alpha-Chl...	5.123	6.018	1915892	5270571	0.865m	1.833 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 14:35
Operator : AJ\MA
Sample : L3308-05
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
5


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:50:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

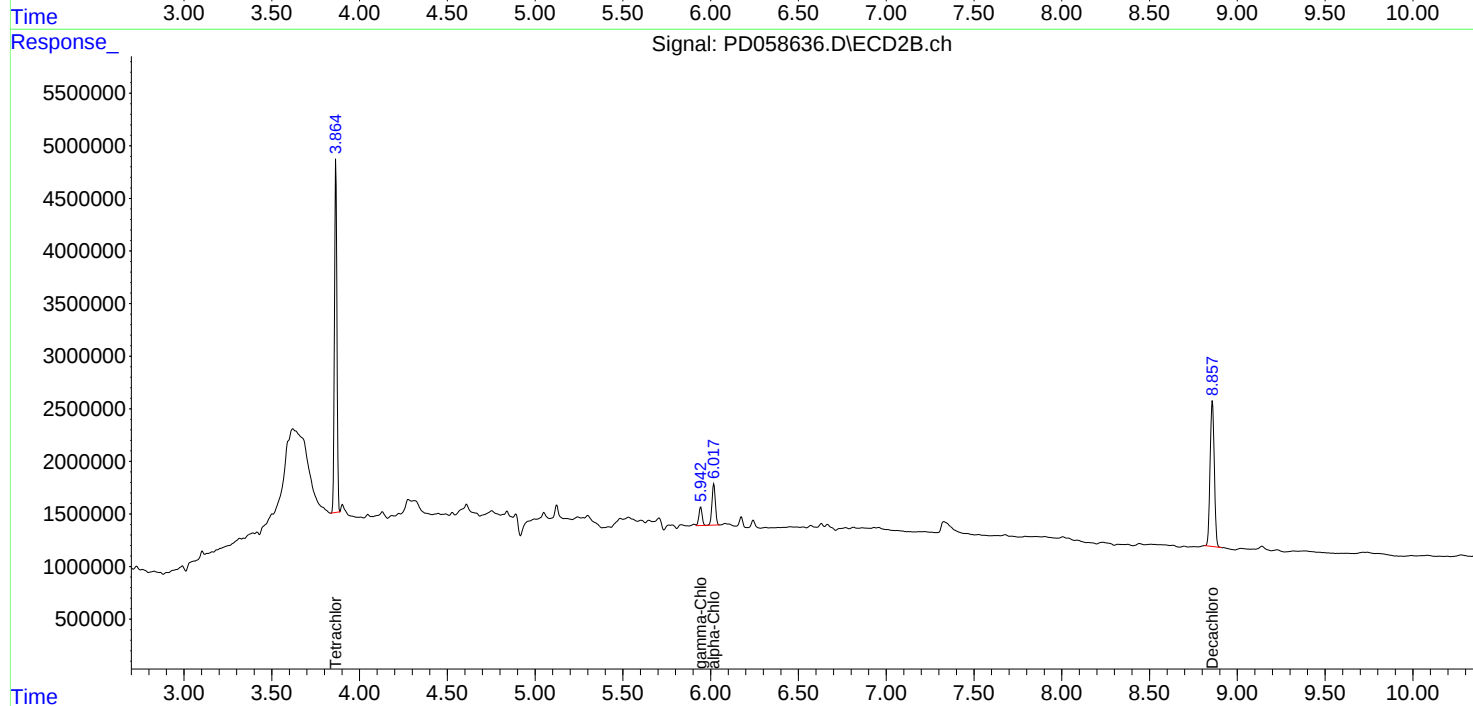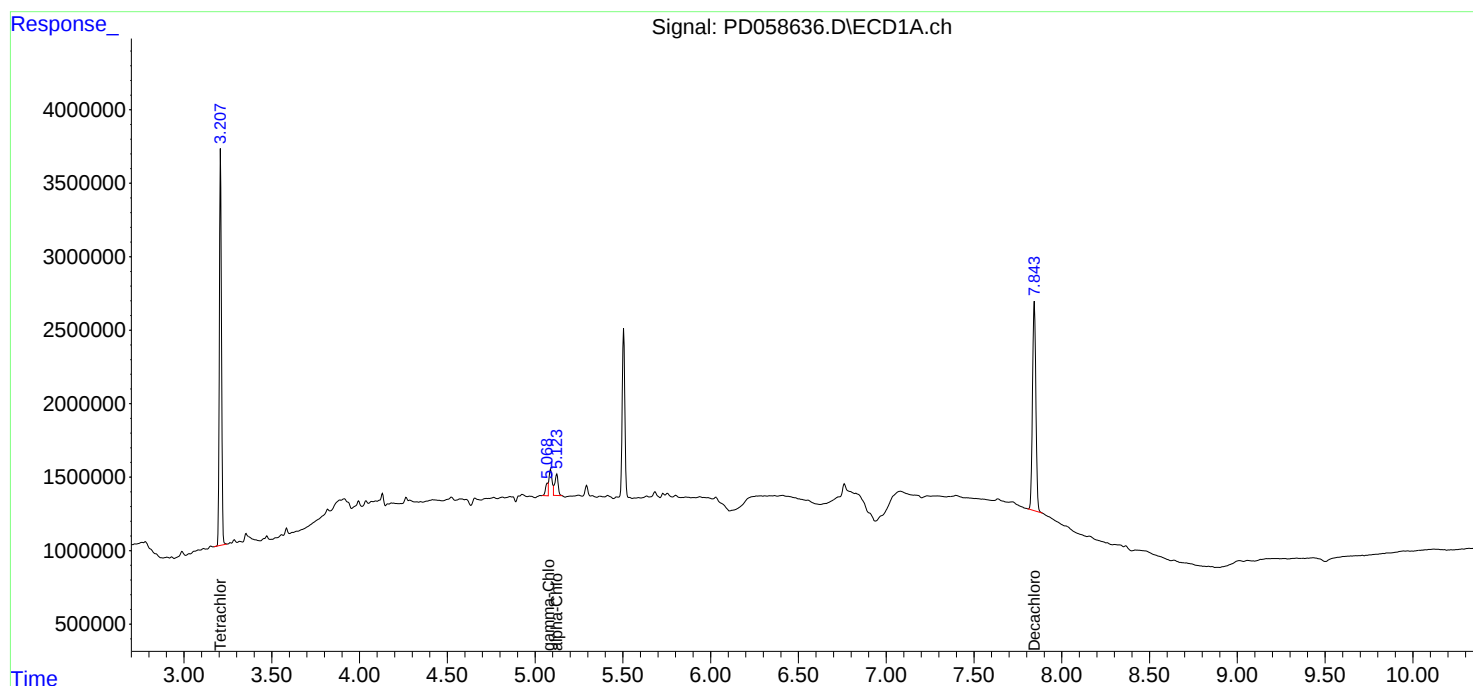

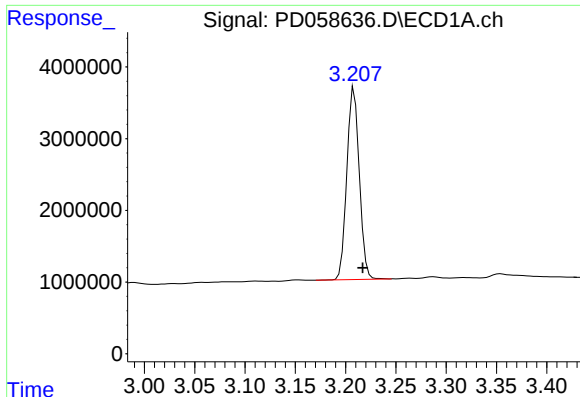


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 23017706
Conc: 12.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
5


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:20 AM

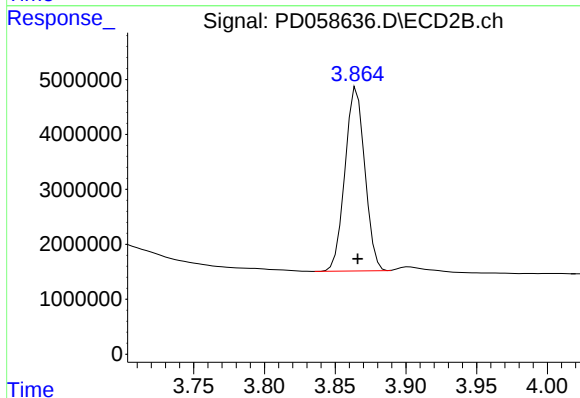


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 32666144
Conc: 13.22 ng/ml

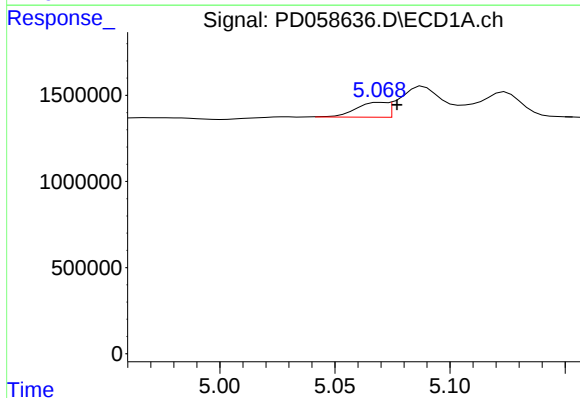


#10 gamma-Chlordane

R.T.: 5.068 min
Delta R.T.: -0.009 min
Response: 905485
Conc: 0.41 ng/ml m

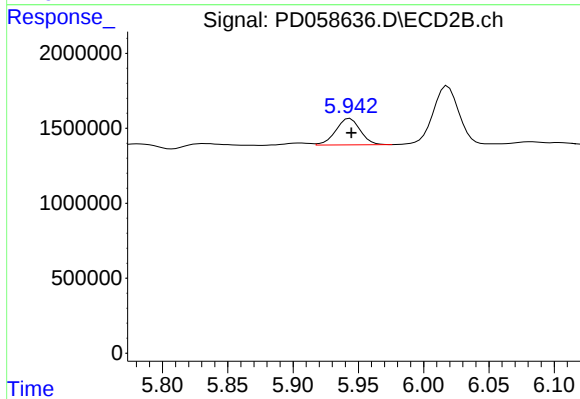

#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.001 min
Response: 2292653
Conc: 0.79 ng/ml

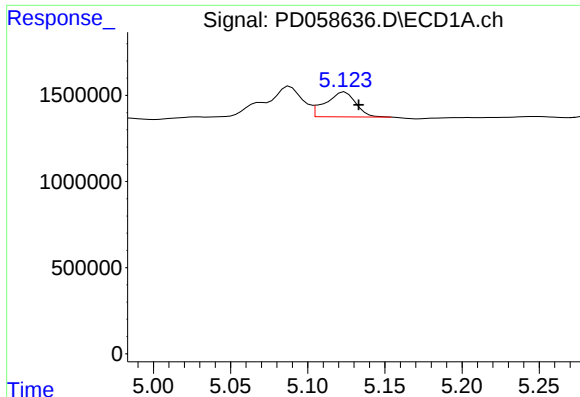


#11 alpha-Chlordane

R.T.: 5.123 min
Delta R.T.: -0.010 min
Response: 1915892
Conc: 0.87 ng/ml m

Instrument :
ECD_D
ClientSampleId :
5


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:20 AM

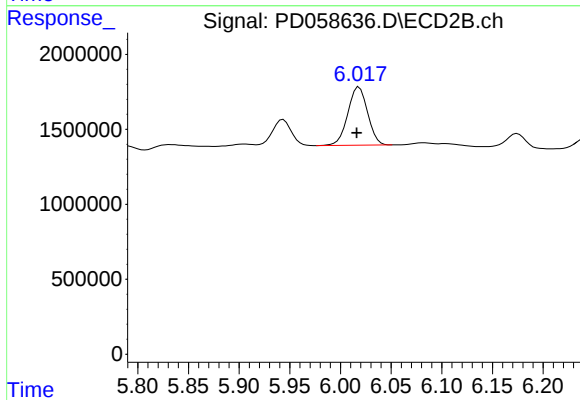


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.002 min
Response: 5270571
Conc: 1.83 ng/ml

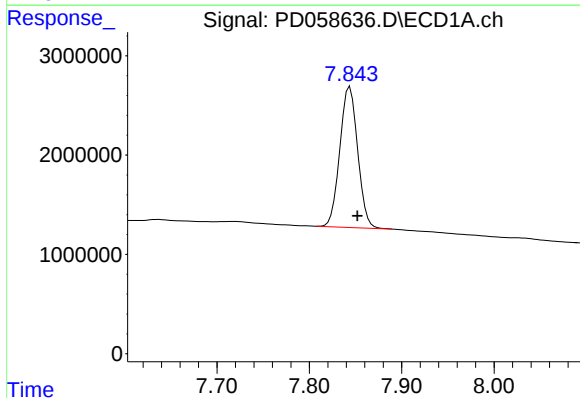

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 18997916
Conc: 10.52 ng/ml

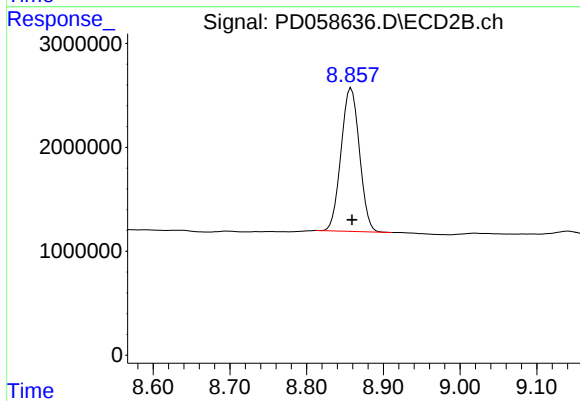

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: -0.001 min
Response: 23052800
Conc: 10.57 ng/ml