

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
 Data File : PD058639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 15:19
 Operator : AJ\MA
 Sample : L3308-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 8

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:42:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 03:51:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.865	21921933	31469810	12.023	12.737
28) SA Decachlor...	7.844	8.858	19045964	23295755	10.547	10.685
Target Compounds						
10) B gamma-Chl...	5.068	5.943	770717	2424270	0.346m	0.833 #
11) B alpha-Chl...	5.122	6.018	2085513	5454447	0.942m	1.897 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071620\
Data File : PD058639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 15:19
Operator : AJ\MA
Sample : L3308-08
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
8


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 03:51:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

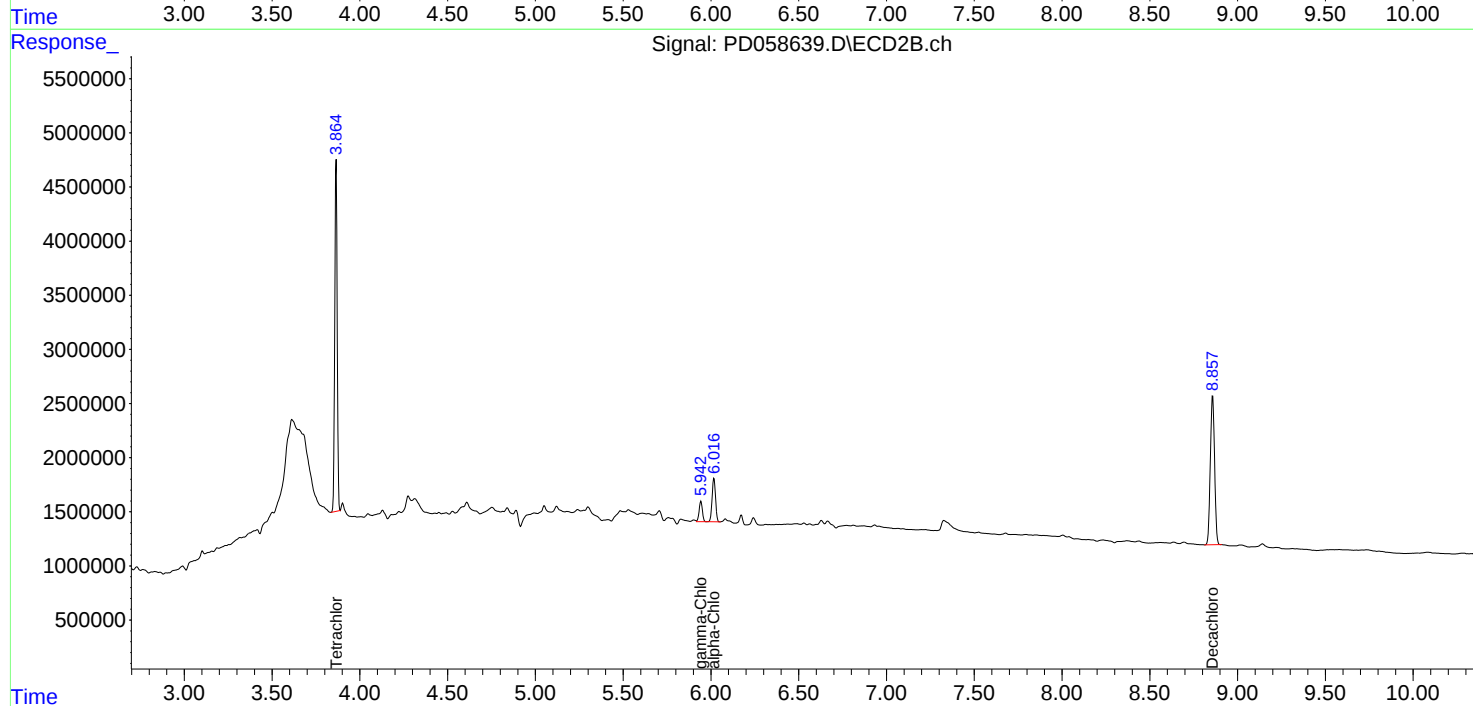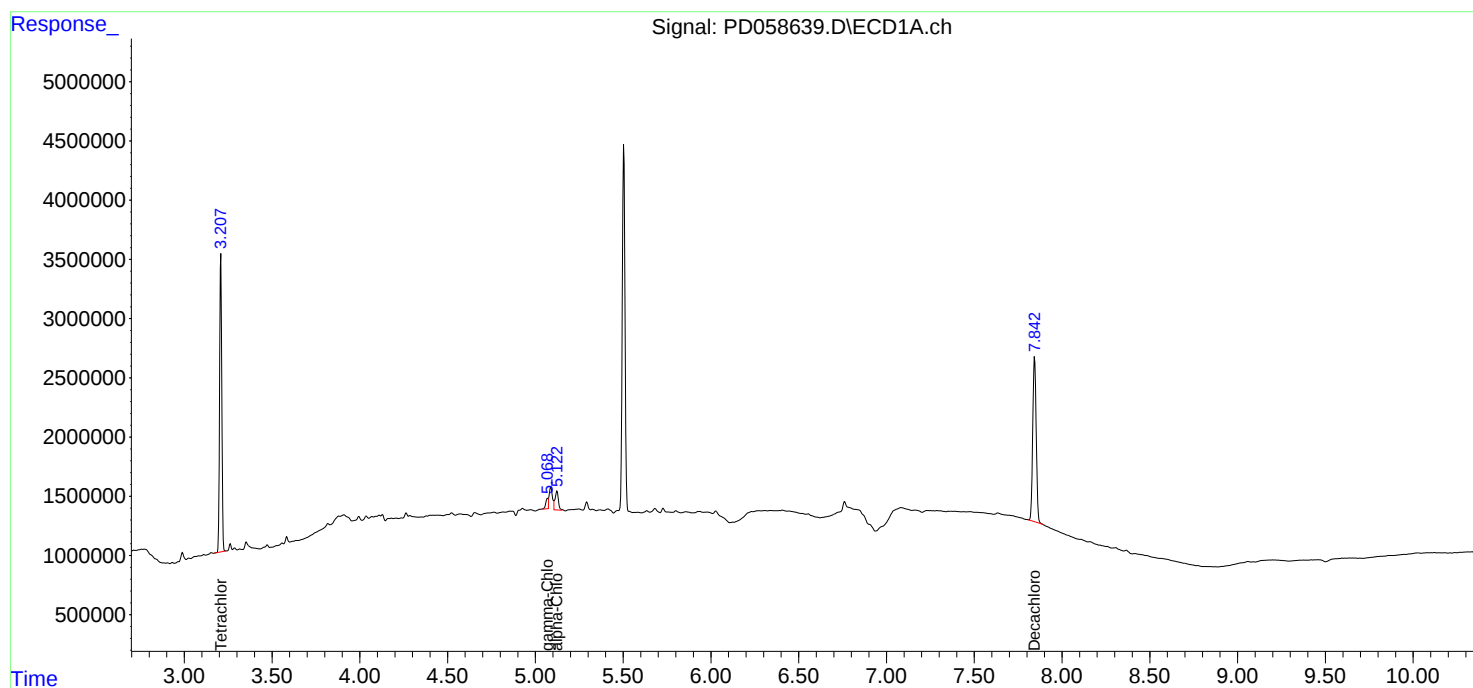

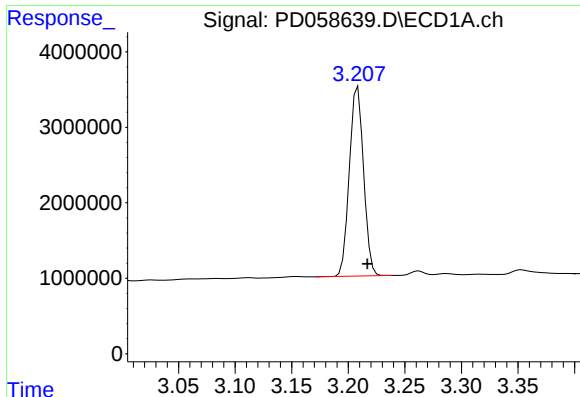


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 21921933
Conc: 12.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
8


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:26 AM

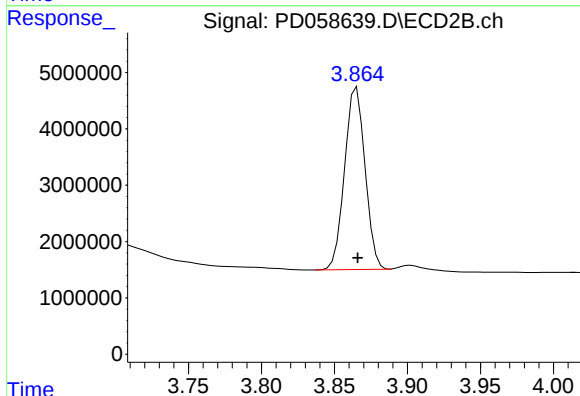


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 31469810
Conc: 12.74 ng/ml

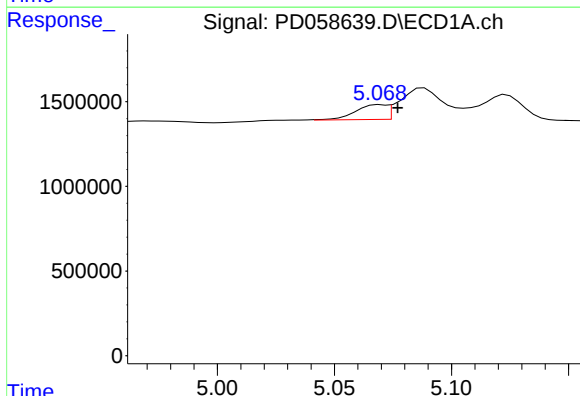


#10 gamma-Chlordane

R.T.: 5.068 min
Delta R.T.: -0.009 min
Response: 770717
Conc: 0.35 ng/ml m

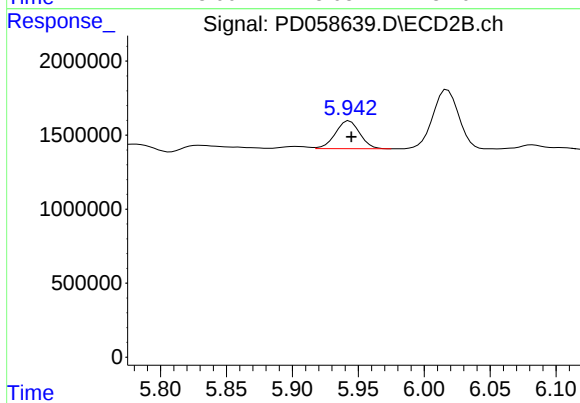

#10 gamma-Chlordane

R.T.: 5.943 min
Delta R.T.: -0.001 min
Response: 2424270
Conc: 0.83 ng/ml

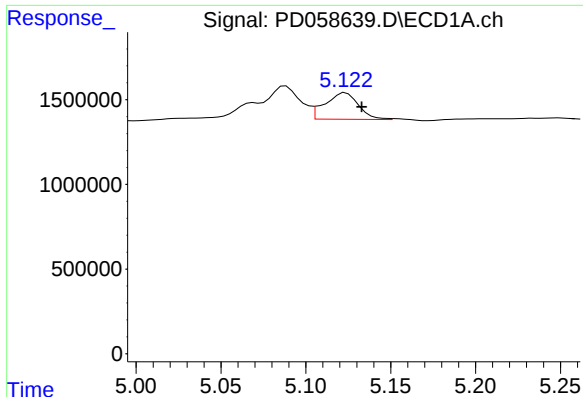


#11 alpha-Chlordane

R.T.: 5.122 min
Delta R.T.: -0.011 min
Response: 2085513
Conc: 0.94 ng/ml m

Instrument :
ECD_D
ClientSampleId :
8


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:26 AM

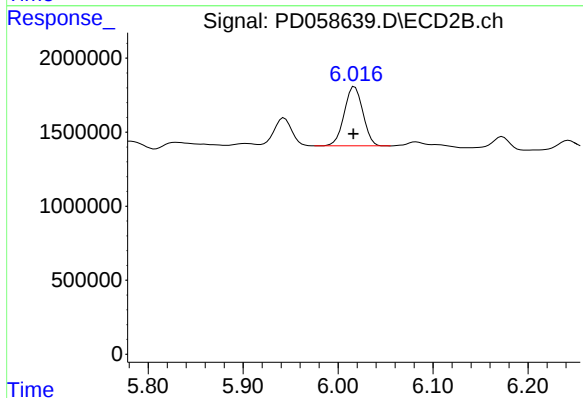


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.001 min
Response: 5454447
Conc: 1.90 ng/ml

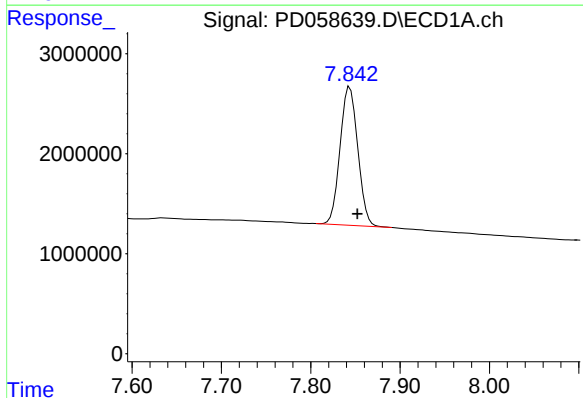

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 19045964
Conc: 10.55 ng/ml

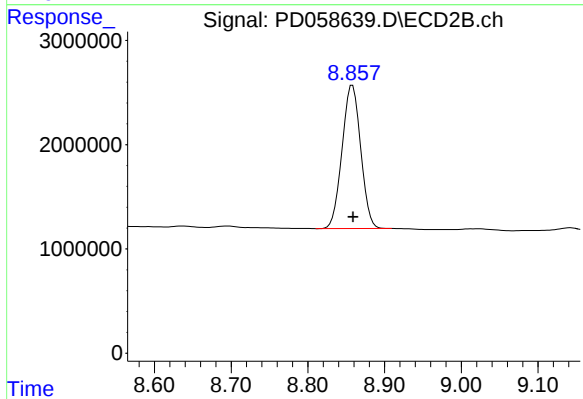

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: -0.001 min
Response: 23295755
Conc: 10.68 ng/ml