

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071621\
 Data File : PD064316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2021 17:25
 Operator : AR\AJ
 Sample : PB137721BS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS721

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 05:23:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 06:42:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.046	3.512	24907789	194.8E6	18.616	19.500
27)	SA Decachlor...	9.209	8.255	57096536	227.4E6	53.238	43.539
Target Compounds							
2)	A alpha-BHC	4.447	3.951	7615687	68034521	4.090	5.087
3)	MA gamma-BHC...	4.738	4.234	7333808	68108434	4.119	5.598 #
4)	MA Heptachlor	5.251	4.533	9292448	65935327	5.268	5.783
5)	MB Aldrin	5.560	4.780	8088523	59432489	5.076	5.738
6)	B beta-BHC	4.917	4.479	5144554	28116551	6.130	5.174
7)	B delta-BHC	5.137	4.684	6990935	51639719	4.093	4.697
8)	B Heptachlo...	5.955	5.222	8408717	51902474	5.516	5.681
9)	A Endosulfan I	6.318	5.560	7770877	51925721	5.624	6.141
10)	B trans-Chl...	6.192	5.447	8130893	54160496	5.144	5.822
11)	B cis-Chlor...	6.265	5.505	8451237	55161215	5.389	6.092
12)	B 4,4'-DDE	6.425	5.667	14794835	97265981	10.680	11.606
13)	MA Dieldrin	6.579	5.804	15568864	93963797	10.749	10.991
14)	MA Endrin	6.800	6.061	13461818	83092982	11.402	11.400
15)	B Endosulfa...	7.016	6.332	14168699	83062243	11.723	12.769
16)	A 4,4'-DDD	6.924	6.182	12033785	77440892	10.568	11.512
17)	MA 4,4'-DDT	7.226	6.422	12605388	70443051	10.920	10.062
18)	B Endrin al...	7.142	6.501	12695067	64579627	12.333	11.661
19)	B Endosulfa...	7.366	6.712	12594303	41184831	10.229	6.689 #
20)	A Methoxychlor	7.690	6.969	37795085	190.8E6	58.904	61.840
21)	B Endrin ke...	7.844	7.206	16637718	78719759	12.519	11.617

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071621\
Data File : PD064316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2021 17:25
Operator : AR\AJ
Sample : PB137721BS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 05:23:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

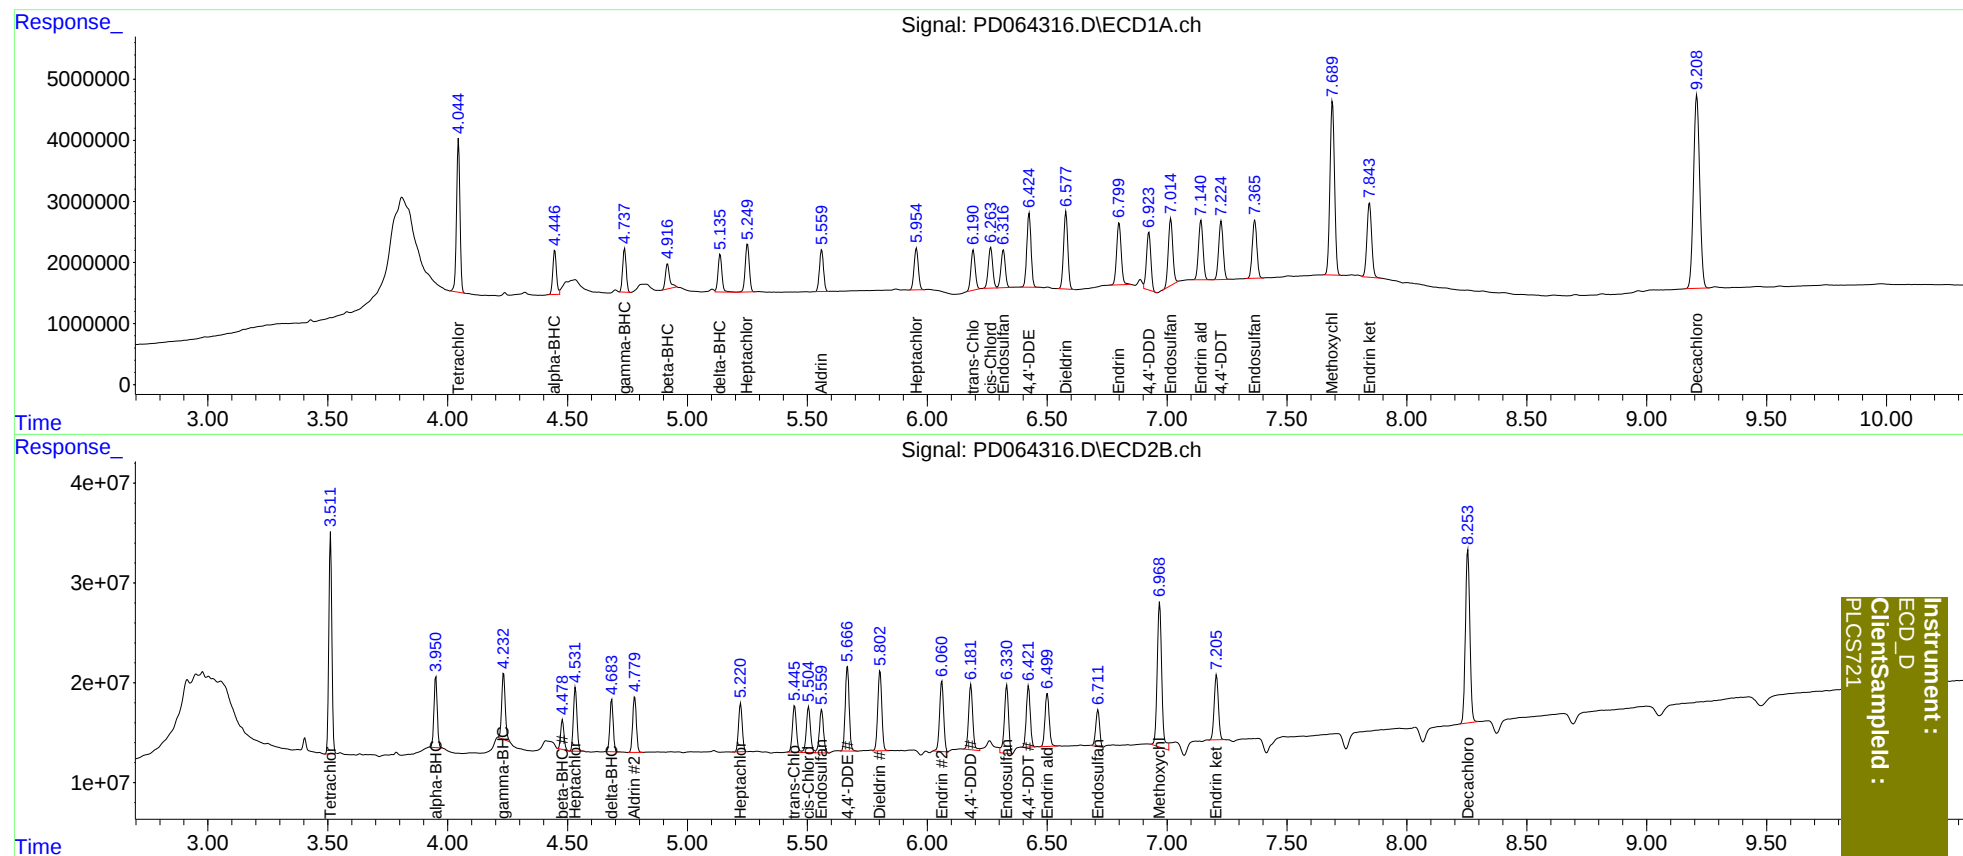

Instrument :
ECD_D
ClientSampled :
PLC5721