

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071621\
 Data File : PD064319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2021 18:07
 Operator : AR\AJ
 Sample : M2995-01MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLX86MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 05:24:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 06:42:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.047	3.512	17369026	107.4E6	12.982	10.745
27)	SA Decachlor...	9.210	8.255	20416674	82898056	19.037	15.869
Target Compounds							
2)	A alpha-BHC	4.447	3.952	91407666	666.7E6	49.094	49.851
3)	MA gamma-BHC...	4.739	4.234	91780829	608.4E6	51.548	50.005
4)	MA Heptachlor	5.251	4.534	97033336	620.8E6	55.006	54.444
5)	MB Aldrin	5.560	4.781	91338130	575.2E6	57.318	55.532
6)	B beta-BHC	4.918	4.480	42770366	268.9E6	50.965	49.485
7)	B delta-BHC	5.137	4.685	28872369	203.3E6	16.904	18.494
8)	B Heptachlo...	5.955	5.223	85598052	495.5E6	56.152	54.231
9)	A Endosulfan I	6.318	5.561	79608471	434.2E6	57.616	51.347
10)	B trans-Chl...	6.192	5.447	85579531	502.6E6	54.144	54.030
11)	B cis-Chlor...	6.265	5.506	85336918	486.6E6	54.420	53.739
12)	B 4,4'-DDE	6.425	5.668	171.2E6	939.4E6	123.594	112.097
13)	MA Dieldrin	6.579	5.804	179.4E6	941.8E6	123.826	110.164
14)	MA Endrin	6.800	6.062	150.0E6	776.8E6	127.074	106.571
15)	B Endosulfa...	7.015	6.332	151.7E6	708.5E6	125.526	108.905
16)	A 4,4'-DDD	6.926	6.183	142.7E6	736.0E6	125.290	109.416
17)	MA 4,4'-DDT	7.226	6.423	152.2E6	755.6E6	131.849	107.925
18)	B Endrin al...	7.142	6.501	131.1E6	606.7E6	127.330	109.545
19)	B Endosulfa...	7.366	6.712	125.4E6	472.3E6	101.833	76.716
20)	A Methoxychlor	7.691	6.969	395.0E6	1579.8E6	615.543	511.949
21)	B Endrin ke...	7.845	7.207	175.8E6	760.9E6	132.262	112.297

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071621\
Data File : PD064319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2021 18:07
Operator : AR\AJ
Sample : M2995-01MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 05:24:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

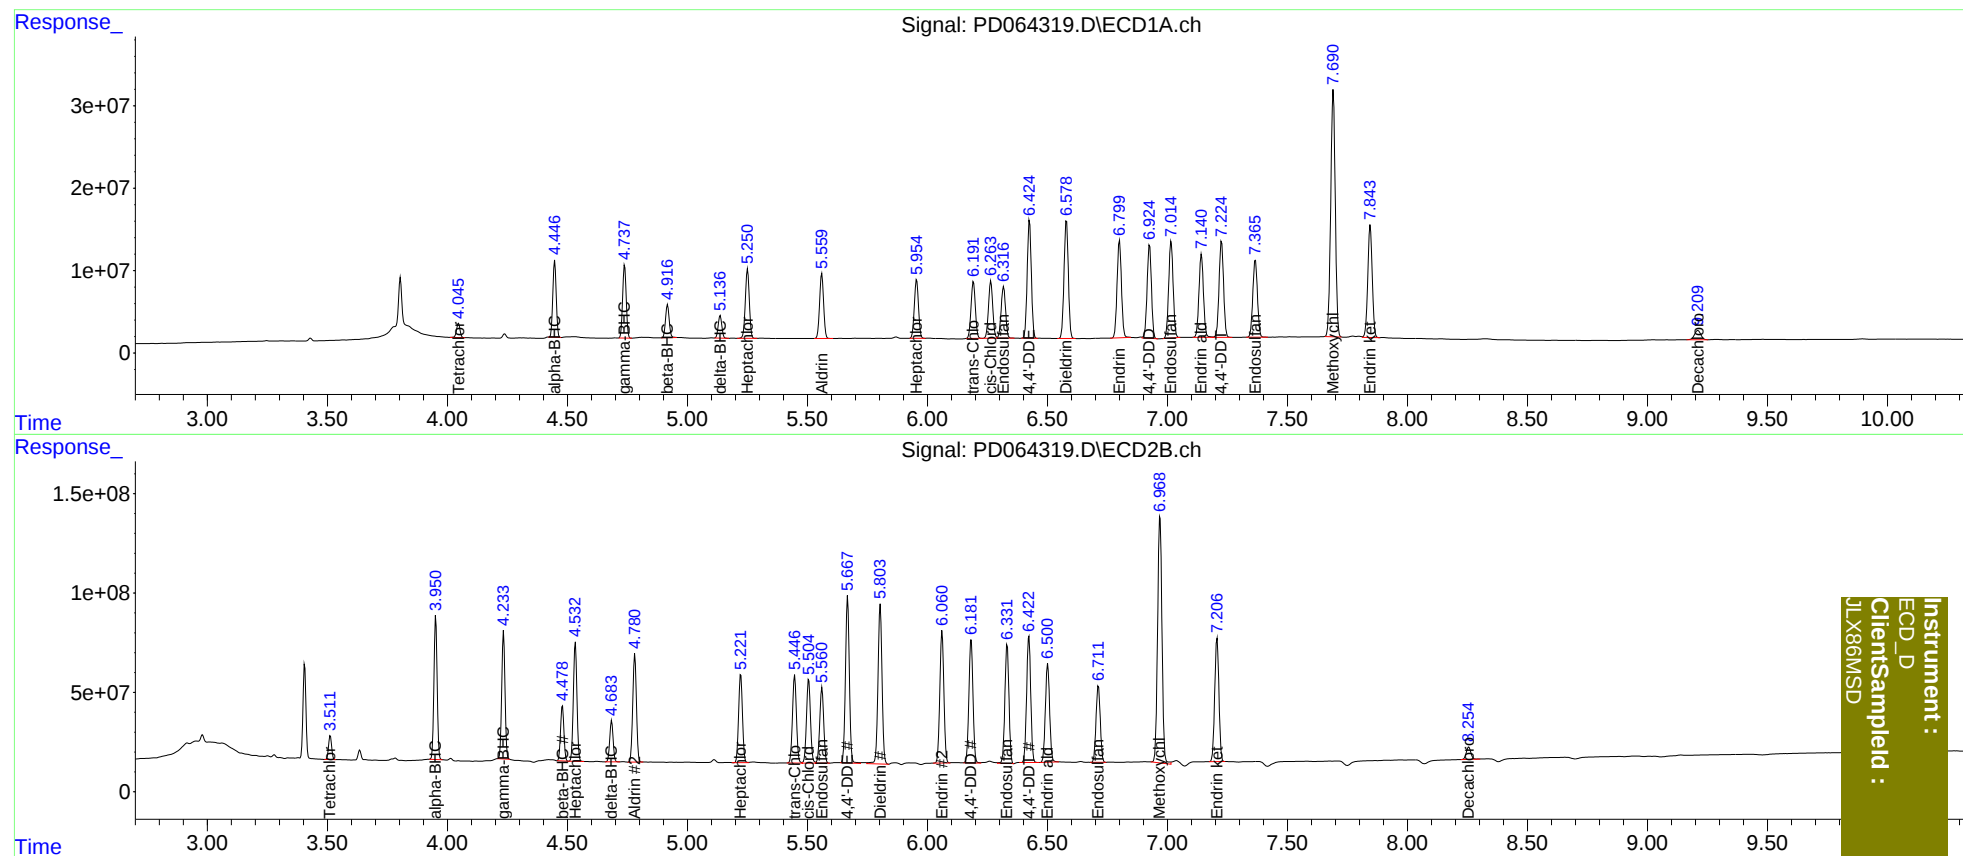

Instrument :
ECD_D
Client Sampled :
JLX86MSD