

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071621\
 Data File : PD064318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2021 17:53
 Operator : AR\AJ
 Sample : M2995-01MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLX86MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 05:23:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 06:42:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.047	3.512	18062651	112.2E6	13.500	11.228
27)	SA Decachlor...	9.210	8.255	21413538	87950308	19.966	16.836
Target Compounds							
2)	A alpha-BHC	4.448	3.952	94715177	696.4E6	50.871	52.074
3)	MA gamma-BHC...	4.739	4.234	95936893	634.4E6	53.882	52.141
4)	MA Heptachlor	5.251	4.533	102.2E6	649.4E6	57.926	56.958
5)	MB Aldrin	5.560	4.781	96390995	599.3E6	60.488	57.859
6)	B beta-BHC	4.918	4.480	44841483	282.8E6	53.433	52.039
7)	B delta-BHC	5.138	4.685	31111700	213.0E6	18.215	19.375
8)	B Heptachlo...	5.956	5.223	90340931	521.3E6	59.264	57.057
9)	A Endosulfan I	6.317	5.561	84323665	452.8E6	61.029	53.555
10)	B trans-Chl...	6.192	5.448	90874961	525.1E6	57.495	56.443
11)	B cis-Chlor...	6.265	5.506	90487172	507.4E6	57.704	56.039
12)	B 4,4'-DDE	6.425	5.668	181.7E6	983.8E6	131.174	117.396
13)	MA Dieldrin	6.579	5.804	189.9E6	985.2E6	131.096	115.239
14)	MA Endrin	6.800	6.062	159.0E6	812.1E6	134.682	111.408
15)	B Endosulfa...	7.016	6.333	161.8E6	751.3E6	133.873	115.493
16)	A 4,4'-DDD	6.925	6.183	151.4E6	766.1E6	132.964	113.889
17)	MA 4,4'-DDT	7.225	6.423	161.1E6	791.1E6	139.568	112.999
18)	B Endrin al...	7.141	6.501	138.3E6	632.9E6	134.381	114.273
19)	B Endosulfa...	7.366	6.713	132.6E6	541.6E6	107.711	87.970
20)	A Methoxychlor	7.690	6.969	414.9E6	1618.3E6	646.661	524.450
21)	B Endrin ke...	7.844	7.207	184.3E6	794.7E6	138.716	117.279

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071621\
Data File : PD064318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2021 17:53
Operator : AR\AJ
Sample : M2995-01MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 05:23:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

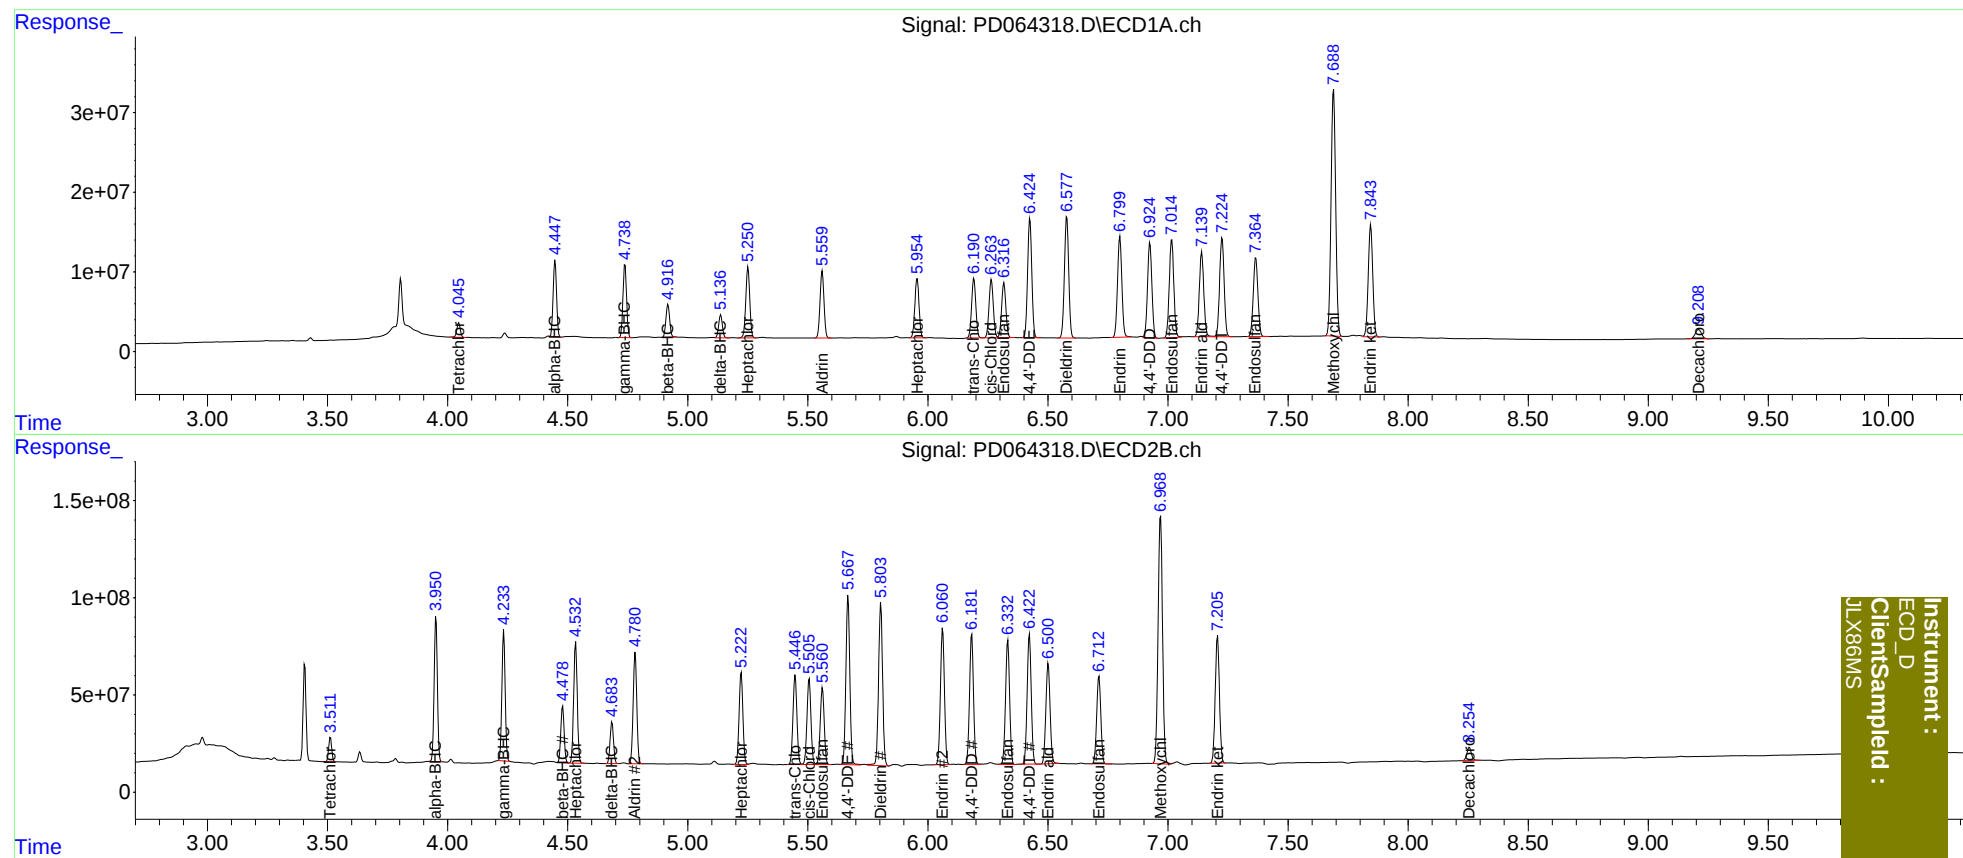

Instrument :
ECD_D
ClientSampled :
JLX86MS