

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
 Data File : PD070937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 17:02
 Operator : AR\AJ
 Sample : N3748-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH0E3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/18/2022
 Supervised By : Ankita Jodhani 07/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 22:20:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.474	4.124	47219169	497.0E6	19.624	21.179
2) SA Decachlor...	8.243	9.319	75297761	280.1E6	29.658	30.330
Target Compounds						
10) B trans-Chl...	5.417	6.281	2547873	16055309	0.732m	1.066 #
11) B cis-Chlor...	5.477	6.356	4440679	17267108	1.299	1.196
13) MA Dieldrin	5.772	6.672	1856468	6437035	0.554m	0.465

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
Data File : PD070937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 17:02
Operator : AR\AJ
Sample : N3748-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 22:20:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

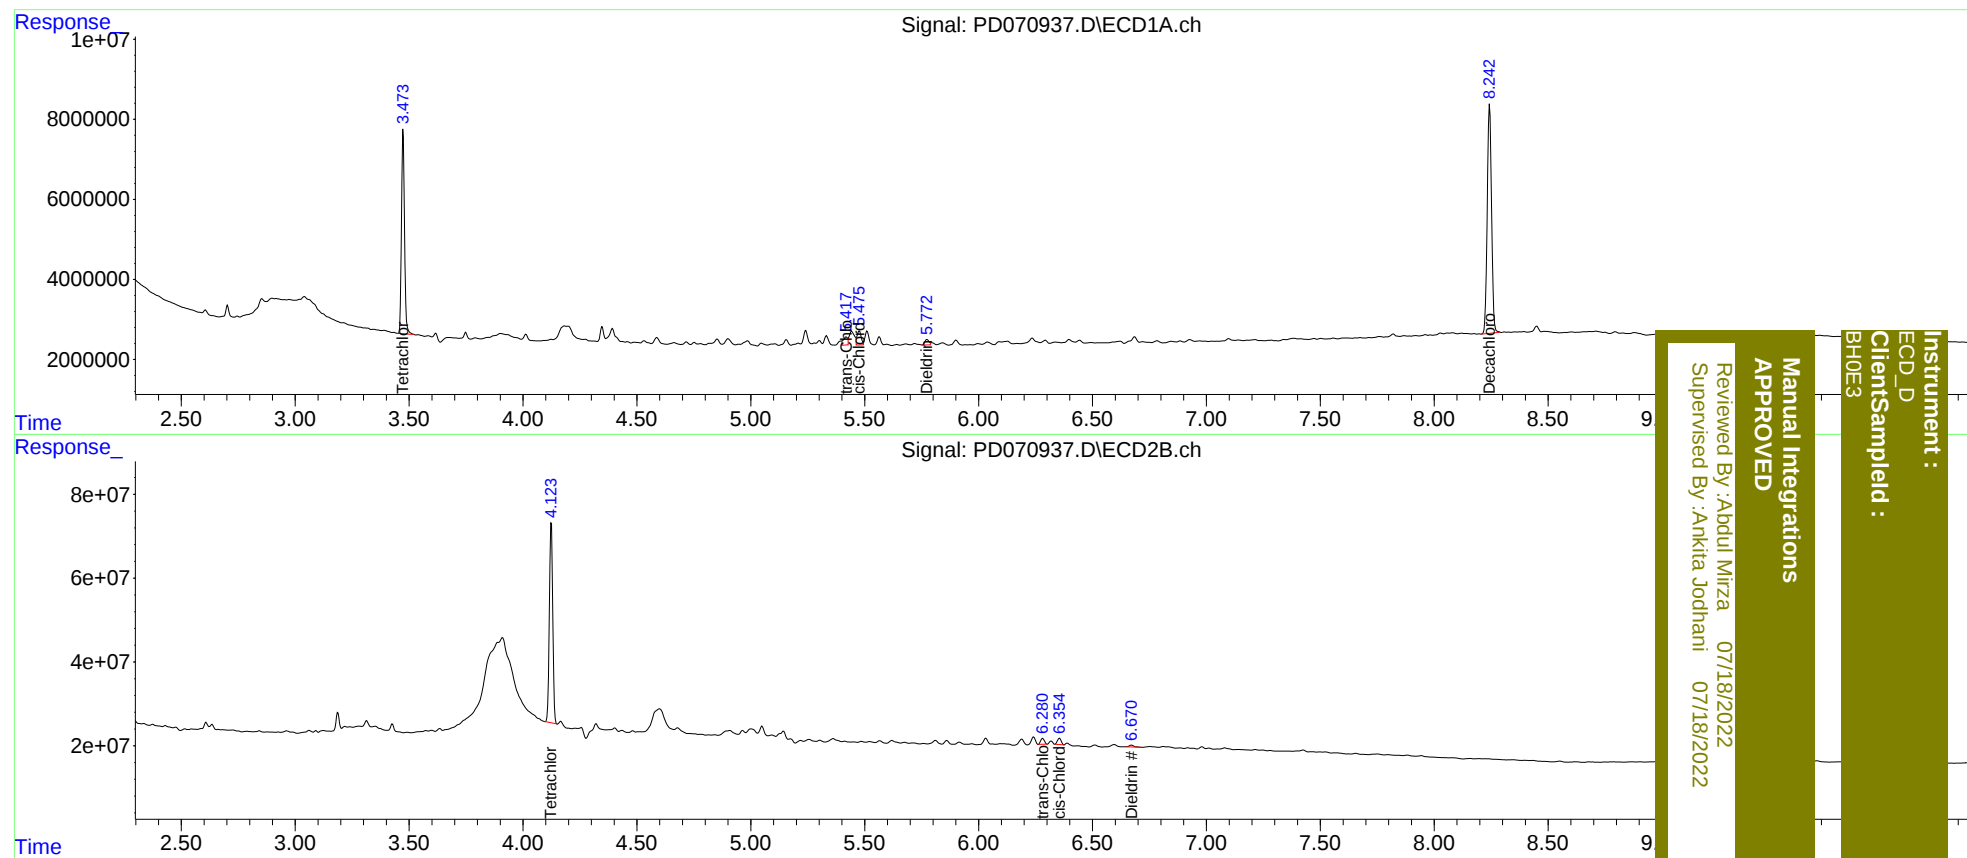

Reviewed By: Abdul Mirza 07/18/2022
Supervised By: Ankita Jodhani 07/18/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BH0E3