

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
 Data File : PD070941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 18:00
 Operator : AR\AJ
 Sample : N3748-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH0E8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/18/2022
 Supervised By :Ankita Jodhani 07/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 22:22:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.123	43913167	461.2E6	18.250	19.654
27)	SA Decachlor...	8.242	9.317	69271848	261.5E6	27.285	28.316
Target Compounds							
10)	B trans-Chl...	5.417	6.281	3107115	14876754	0.893m	0.988
11)	B cis-Chlor...	5.476	6.354	4203696	16453250	1.230	1.139
13)	MA Dieldrin	5.771	6.672	1960701	6662735	0.586m	0.481

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
Data File : PD070941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 18:00
Operator : AR\AJ
Sample : N3748-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 22:22:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

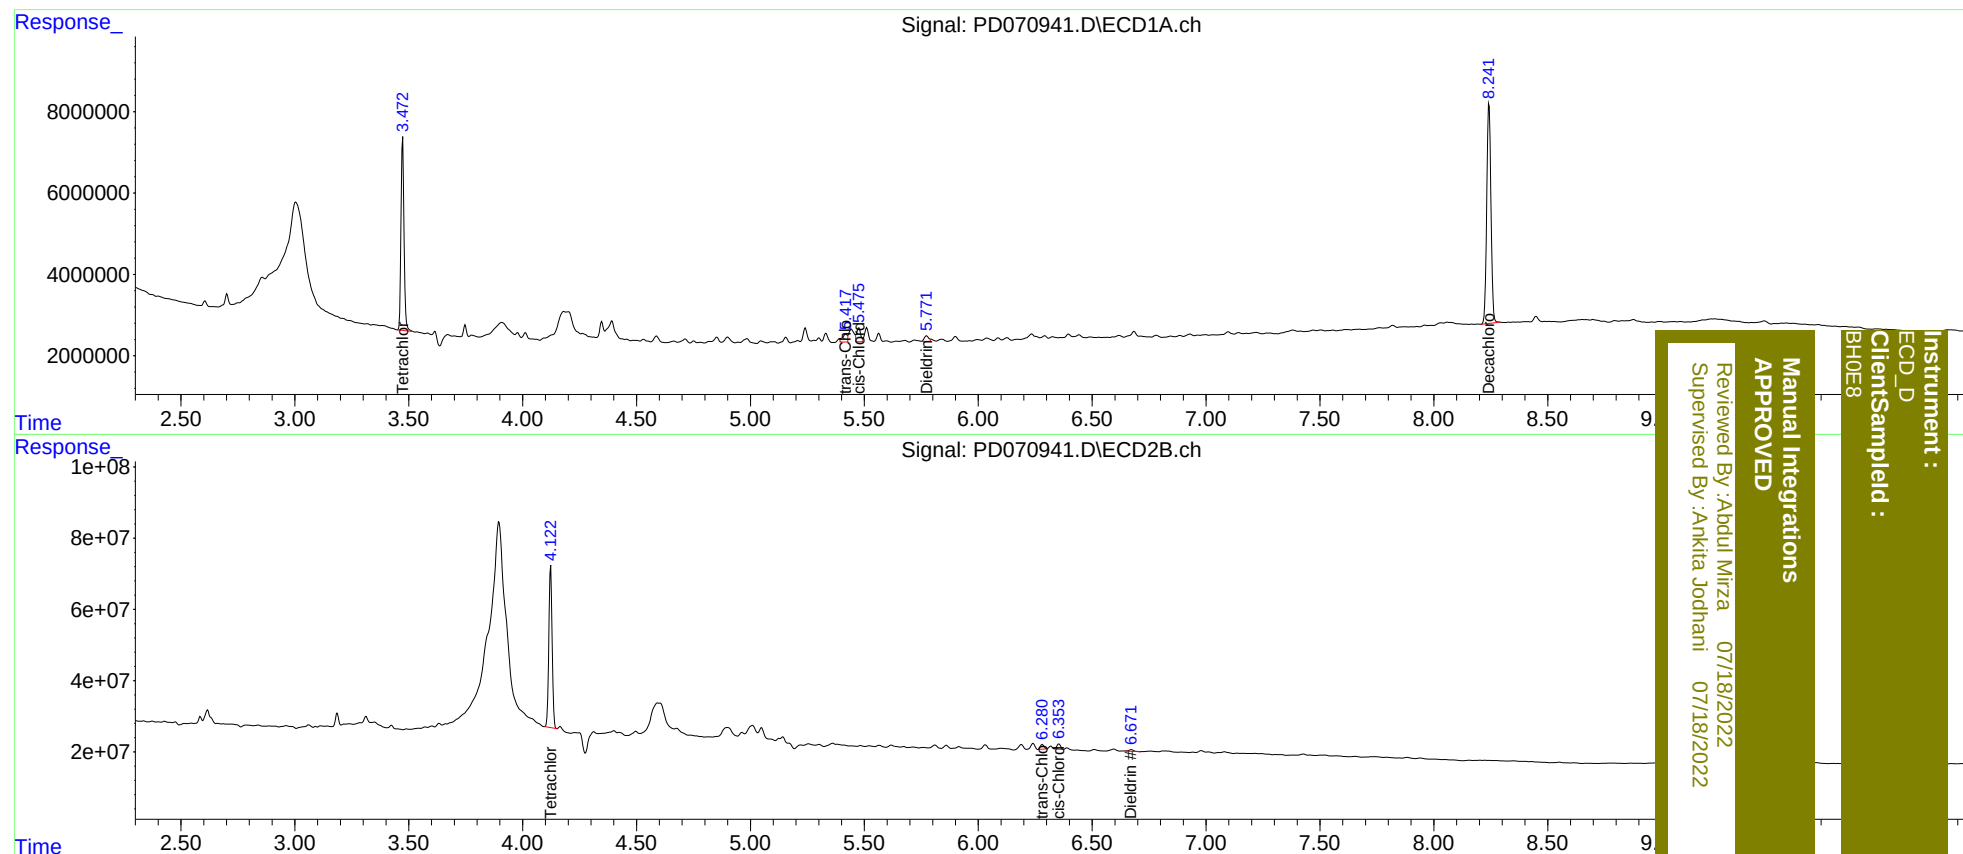

Reviewed By: Abdul Mirza 07/18/2022
Supervised By: Ankita Jodhani 07/18/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BH0E8