

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
 Data File : PD070943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 18:29
 Operator : AR\AJ
 Sample : N3748-08MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH0E9MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 22:22:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.123	42081498	434.5E6	17.489	18.514
27)	SA Decachlor...	8.242	9.318	57221464	212.5E6	22.538	23.005
Target Compounds							
2)	A alpha-BHC	3.914	4.529	191.9E6	1430.3E6	51.168	47.388
3)	MA gamma-BHC...	4.198	4.822	177.8E6	1234.5E6	48.853	47.706
4)	MA Heptachlor	4.498	5.338	173.3E6	871.3E6	49.745	43.475
5)	MB Aldrin	4.747	5.651	177.7E6	757.9E6	49.185	43.548
6)	B beta-BHC	4.447	4.998	69930387	484.0E6	44.636	36.189
7)	B delta-BHC	4.653	5.222	175.4E6	1006.4E6	50.347	44.370
8)	B Heptachlo...	5.192	6.046	160.1E6	634.5E6	48.097	42.725
9)	A Endosulfan I	5.532	6.410	147.5E6	563.8E6	48.928	42.514
10)	B trans-Chl...	5.419	6.282	166.5E6	629.0E6	47.855	41.771
11)	B cis-Chlor...	5.478	6.355	161.2E6	599.8E6	47.160	41.525
12)	B 4,4'-DDE	5.643	6.510	307.4E6	1182.8E6	95.529	86.237
13)	MA Dieldrin	5.776	6.671	341.3E6	1275.1E6	101.930	92.085
14)	MA Endrin	6.034	6.894	296.9E6	1047.2E6	107.080	100.292
15)	B Endosulfa...	6.308	7.109	273.5E6	1032.6E6	99.741	89.645
16)	A 4,4'-DDD	6.161	7.010	250.0E6	993.0E6	96.007	90.794
17)	MA 4,4'-DDT	6.402	7.311	275.8E6	1085.9E6	103.088	97.031
18)	B Endrin al...	6.478	7.234	189.6E6	764.8E6	82.773	78.664
19)	B Endosulfa...	6.690	7.458	255.9E6	966.4E6	91.344	85.241
20)	A Methoxychlor	6.953	7.771	679.1E6	2436.3E6	491.092	465.643
21)	B Endrin ke...	7.184	7.940	306.3E6	1126.0E6	98.809	91.188

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
Data File : PD070943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 18:29
Operator : AR\AJ
Sample : N3748-08MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 22:22:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

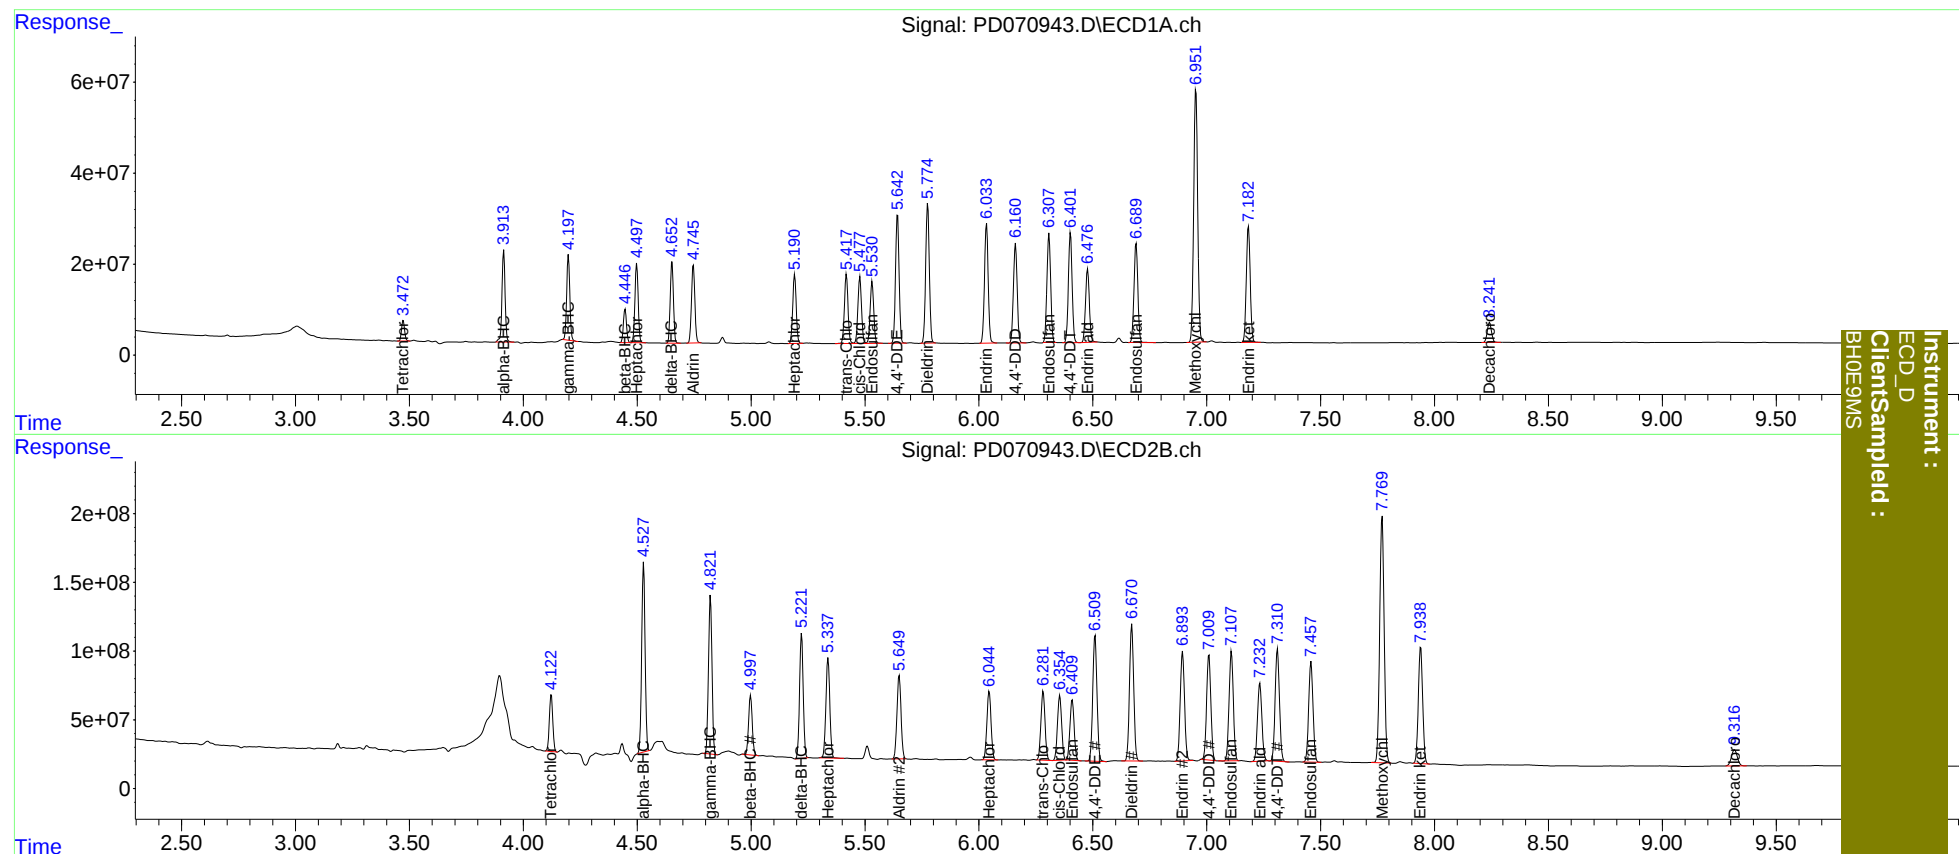

Instrument :
ECD_D
ClientSampled :
BH0E9MS