

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
 Data File : PD070952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 21:24
 Operator : AR\AJ
 Sample : N3704-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/18/2022
 Supervised By :Ankita Jodhani 07/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 22:25:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.123	44875397	440.4E6	18.650	18.765
27)	SA Decachlor...	8.241	9.316	58682916	221.9E6	23.114	24.022
Target Compounds							
15)	B Endosulfa...	6.322	7.105	3415035	14087337	1.245m	1.223

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071622\
Data File : PD070952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 21:24
Operator : AR\AJ
Sample : N3704-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 22:25:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

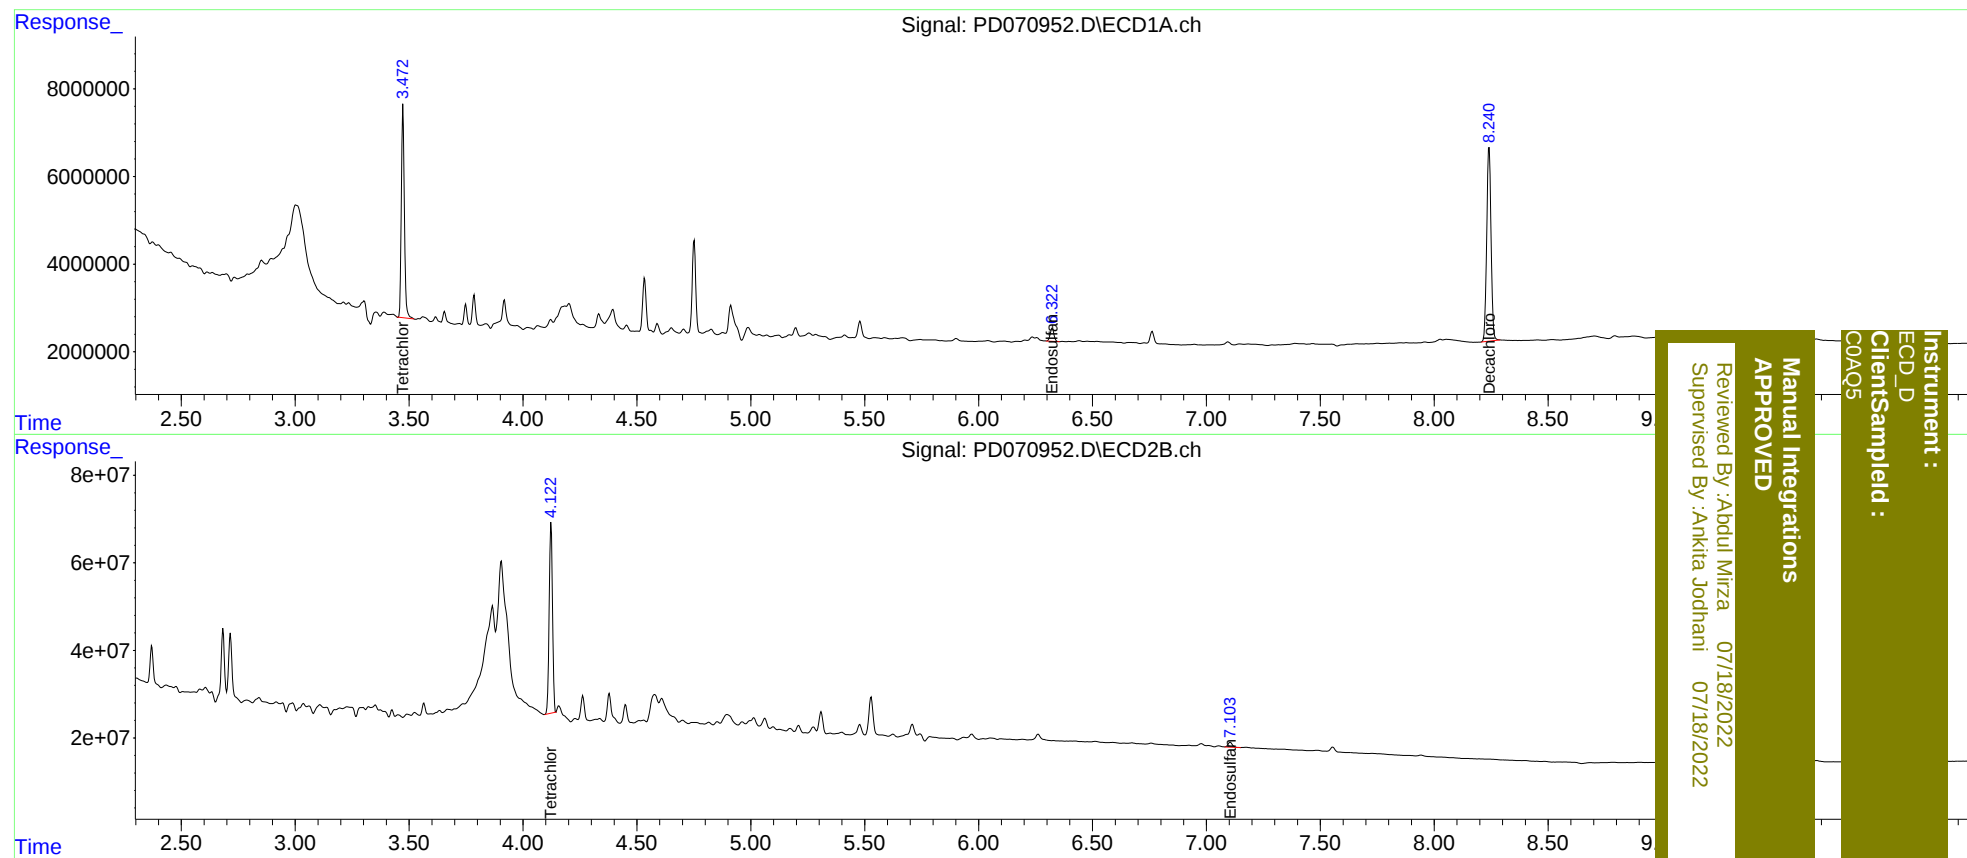

Instrument :
ECD_D
ClientSampled :
COA05

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/18/2022
Supervised By :Ankita Jodhani 07/18/2022

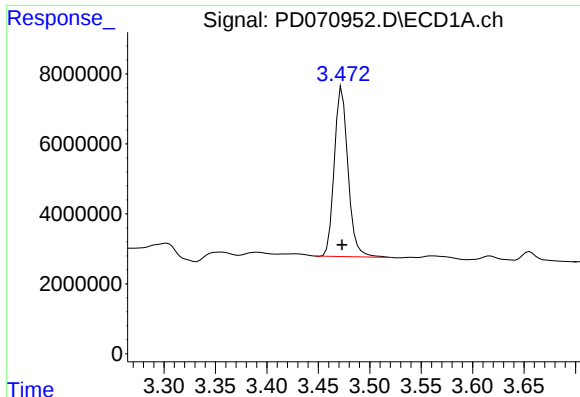


#1 Tetrachloro-m-xylene

R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 44875397
Conc: 18.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/18/2022
Supervised By :Ankita Jodhani 07/18/2022

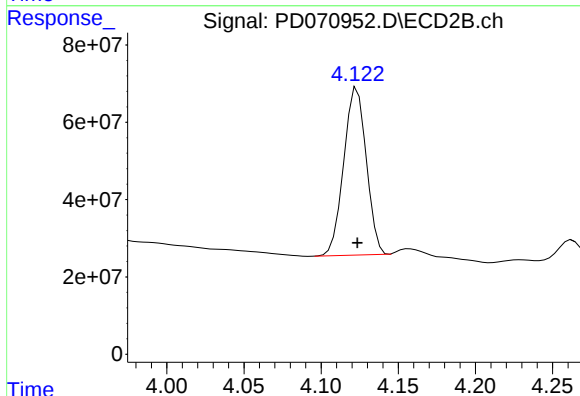


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 440379321
Conc: 18.76 ng/ml

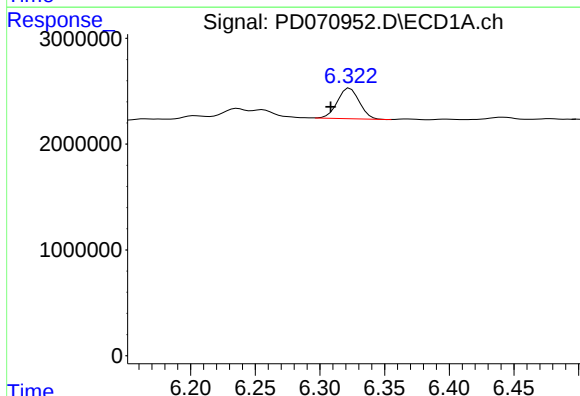


#15 Endosulfan II

R.T.: 6.322 min
Delta R.T.: 0.013 min
Response: 3415035
Conc: 1.25 ng/ml m

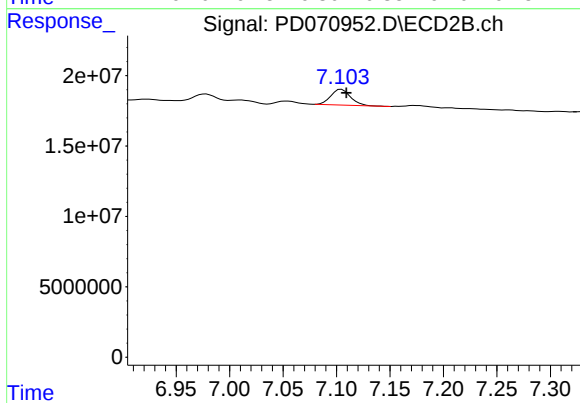

#15 Endosulfan II

R.T.: 7.105 min
Delta R.T.: -0.005 min
Response: 14087337
Conc: 1.22 ng/ml

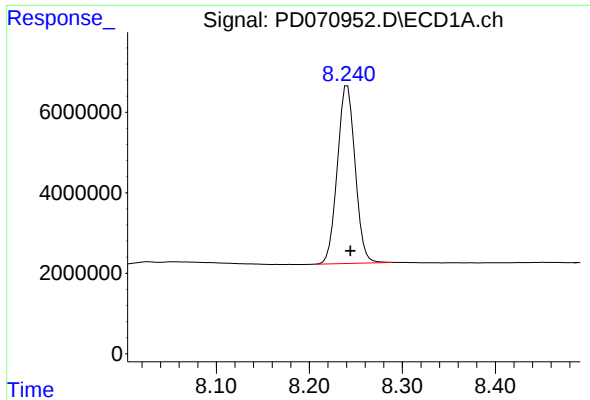


#27 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: -0.003 min
Response: 58682916
Conc: 23.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ5

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/18/2022
Supervised By :Ankita Jodhani 07/18/2022

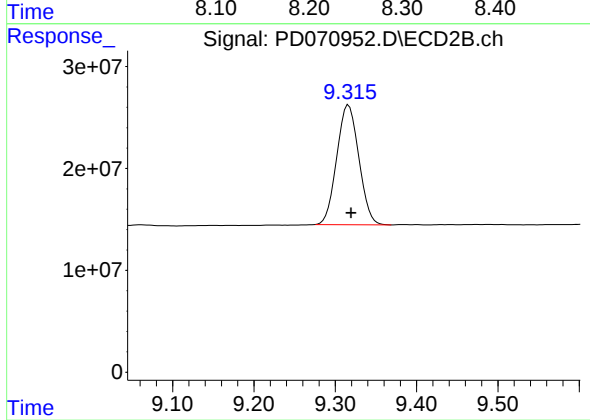

#27 Decachlorobiphenyl

R.T.: 9.316 min
Delta R.T.: -0.003 min
Response: 221857673
Conc: 24.02 ng/ml