

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071624\
 Data File : PD083960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 18:31
 Operator : AR\AJ
 Sample : P3217-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 YDZH6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:32:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.772	21416017	113.7E6	21.093	20.980
2)	SA Decachlor...	9.116	7.897	45194182	132.9E6	21.211	19.888
Target Compounds							
2)	A alpha-BHC	4.068f	0.000	130183	0	<MDL	N.D. #
7)	B delta-BHC	4.790	0.000	1000552	0	0.472	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071624\
Data File : PD083960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 18:31
Operator : AR\AJ
Sample : P3217-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:32:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

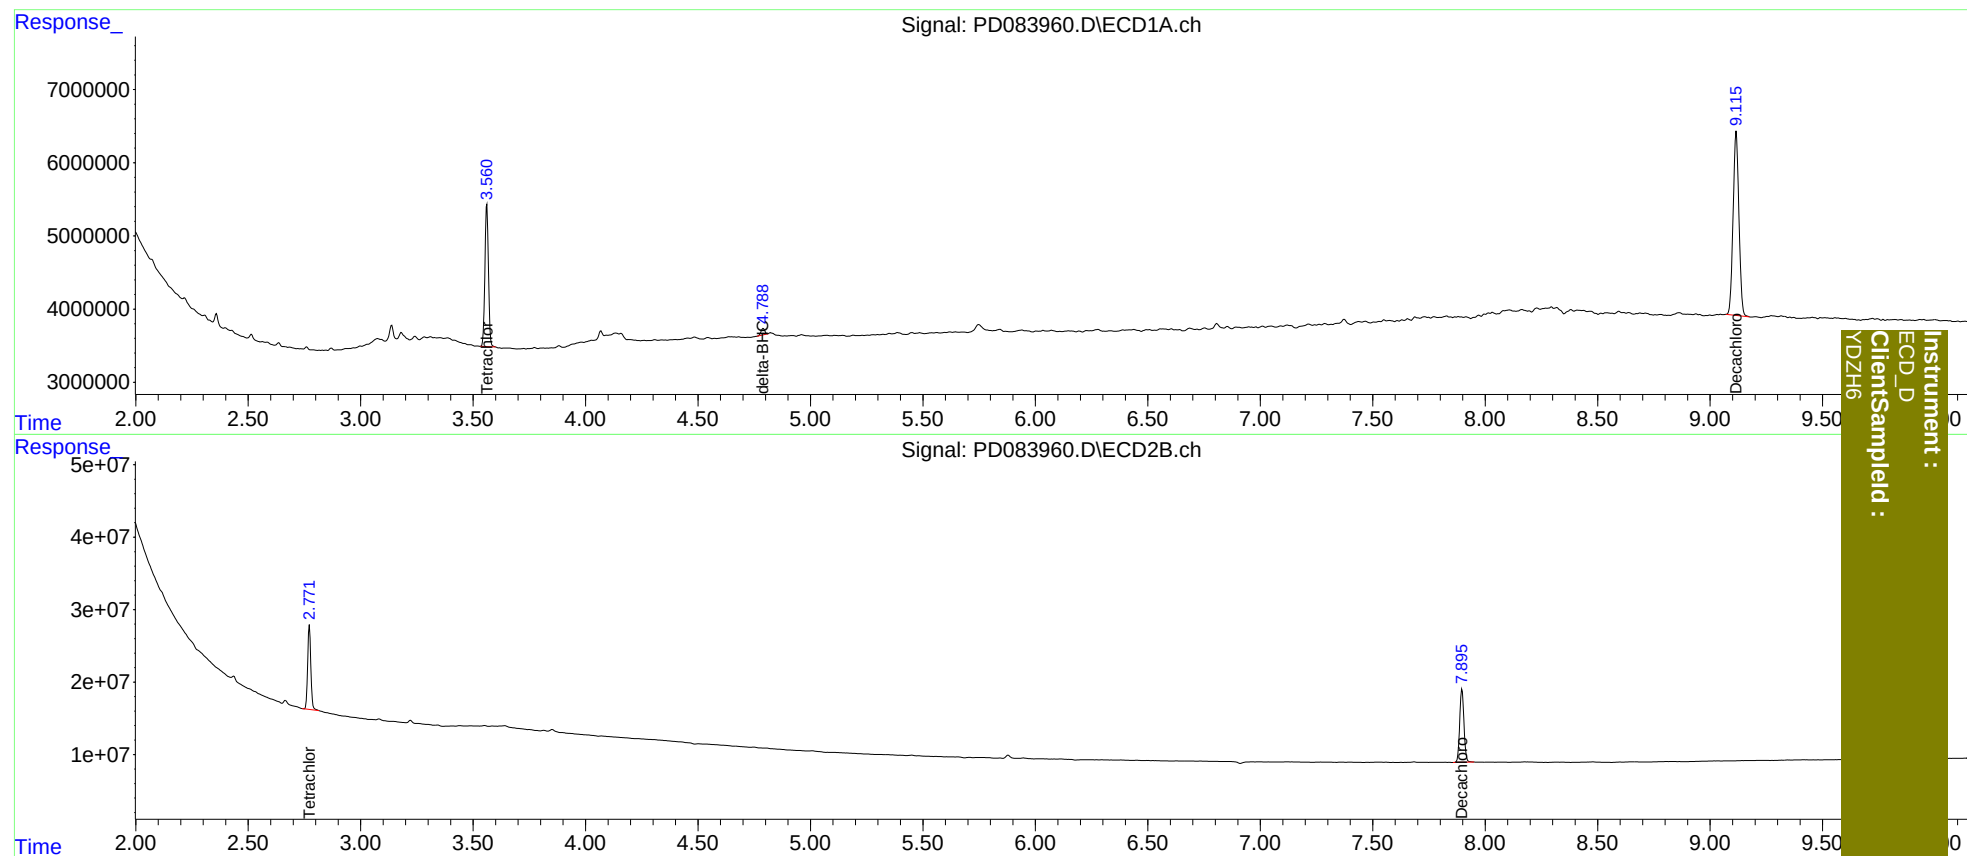


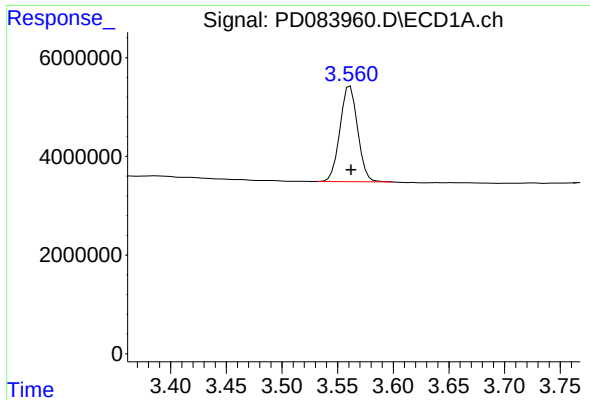

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 21416017
Conc: 21.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
YDZH6

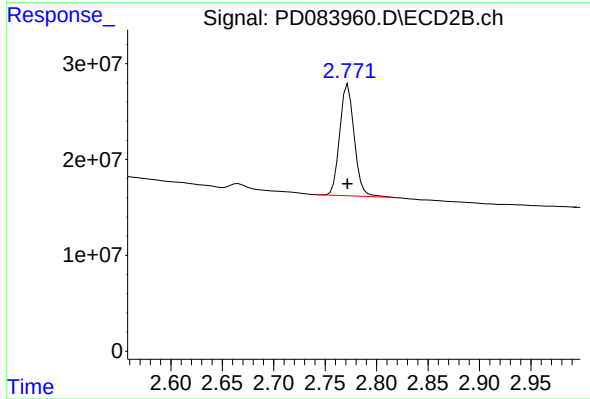


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 113703917
Conc: 20.98 ng/ml

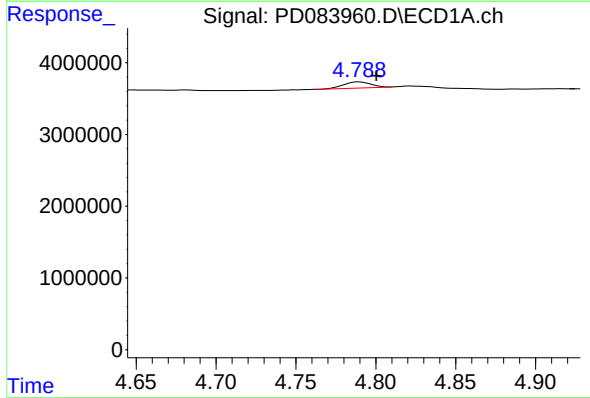


#7 delta-BHC

R.T.: 4.790 min
Delta R.T.: -0.010 min
Response: 1000552
Conc: 0.47 ng/ml

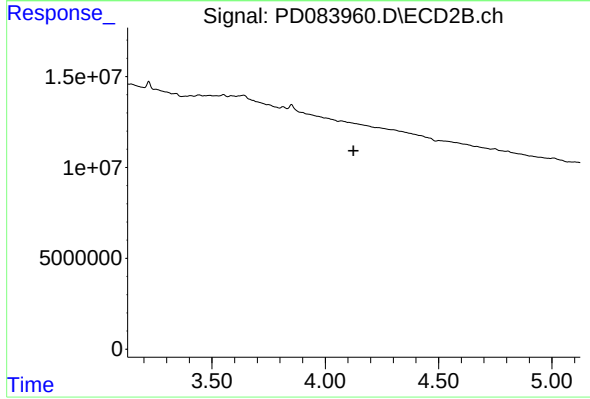

#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.125 min
Response: 0
Conc: N.D.

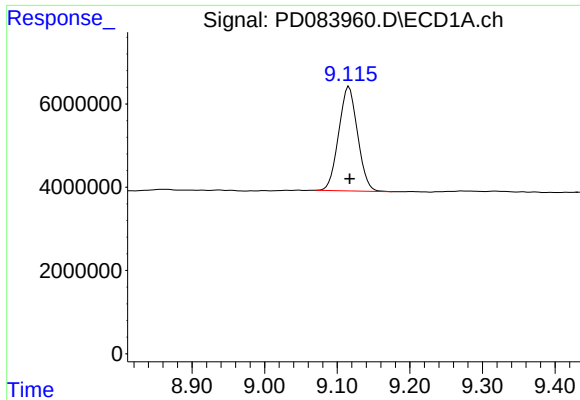

#27 Decachlorobiphenyl


R.T.: 9.116 min

Delta R.T.: -0.001 min

Response: 45194182

Conc: 21.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
YDZH6

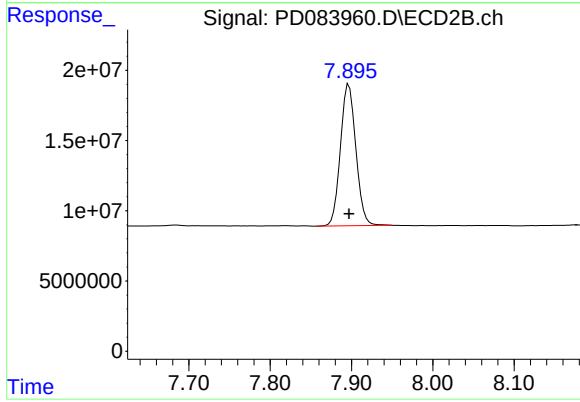

#27 Decachlorobiphenyl

R.T.: 7.897 min

Delta R.T.: 0.000 min

Response: 132872530

Conc: 19.89 ng/ml