

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
 Data File : PD076811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 10:17
 Operator : AR\AJ
 Sample : 03418-23MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46K6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 13:46:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.763	104.5E6	15264800	49.110m	14.301m#
27)	SA Decachlor...	9.083	7.904	56057096	25791947	23.074	24.060
Target Compounds							
2)	A alpha-BHC	3.999	3.266	204.1E6	87691761	57.584m	55.418
3)	MA gamma-BHC...	4.335	3.594	299.6E6	84794969	90.332m	56.601m#
4)	MA Heptachlor	4.924	3.934	177.4E6	146.8E6	51.040m	98.160 #
5)	MB Aldrin	5.268	4.215	188.7E6	121.5E6	55.174	80.715 #
6)	B beta-BHC	4.523	3.892	65194415	29608193	42.892m	41.330
7)	B delta-BHC	4.780	4.122	216.1E6	92491908	64.456m	60.599
8)	B Heptachlo...	5.695	4.717	166.0E6	77847861	55.396	55.334
9)	A Endosulfan I	6.082	5.087	149.6E6	63196752	52.523	51.007
10)	B trans-Chl...	5.952	4.967	158.9E6	73316407	51.677	54.219
11)	B cis-Chlor...	6.031	5.031	162.9E6	71651016	51.378	50.787
12)	B 4,4'-DDE	6.204	5.220	305.9E6	139.8E6	105.001	115.655
13)	MA Dieldrin	6.358	5.352	340.8E6	158.5E6	108.018	113.649
14)	MA Endrin	6.588	5.627	277.8E6	125.7E6	107.755	101.651
15)	B Endosulfa...	6.807	5.921	270.9E6	131.5E6	101.872m	109.335
16)	A 4,4'-DDD	6.722	5.775	267.1E6	111.8E6	118.216	118.008
17)	MA 4,4'-DDT	7.035	6.025	236.9E6	102.8E6	106.080m	109.741
18)	B Endrin al...	6.938	6.101	159.4E6	70148289	85.236	83.628
19)	B Endosulfa...	7.173	6.324	258.2E6	115.9E6	103.396	103.909
20)	A Methoxychlor	7.513	6.601	619.2E6	243.1E6	467.759	455.567
21)	B Endrin ke...	7.660	6.829	312.2E6	128.8E6	112.740	100.660m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
Data File : PD076811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 10:17
Operator : AR\AJ
Sample : 03418-23MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 13:46:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

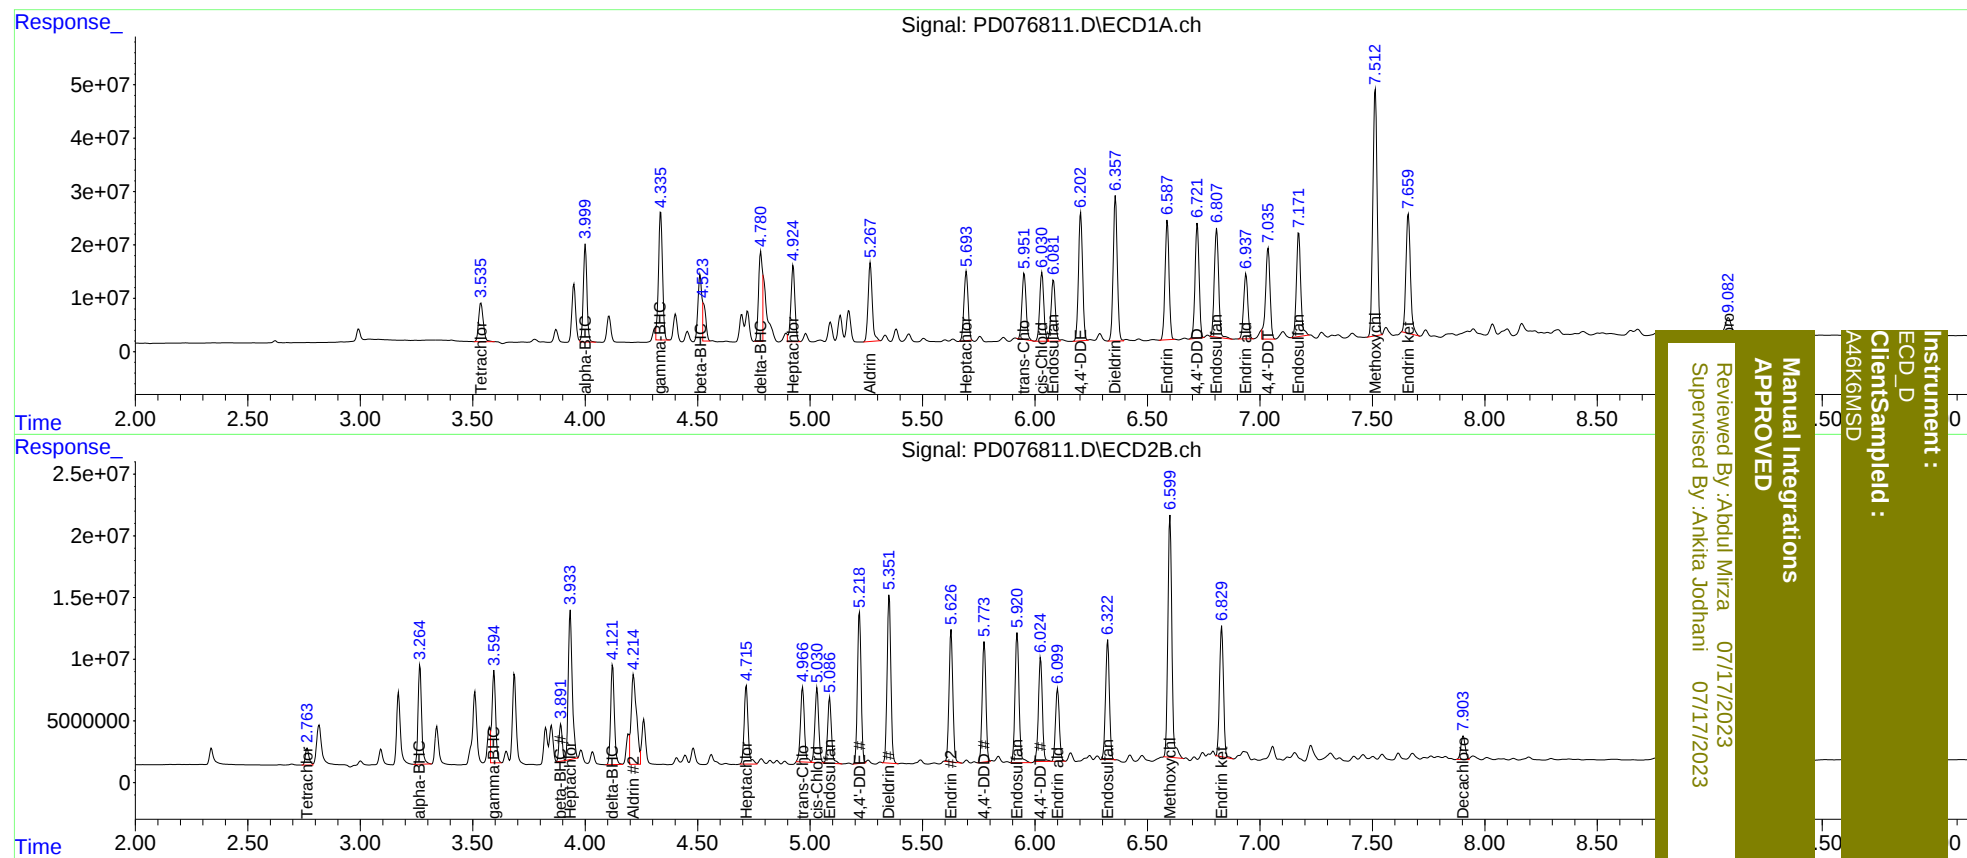

Reviewed By: Abdul Miza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
A46K6MSD