

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
 Data File : PD076810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 10:04
 Operator : AR\AJ
 Sample : 03418-22MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46K6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 13:46:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.763	104.3E6	15321028	49.016m	14.353m#
27)	SA Decachlor...	9.084	7.905	56379029	25713620	23.206	23.987
Target Compounds							
2)	A alpha-BHC	4.000	3.265	202.5E6	87201702	57.128m	55.109
3)	MA gamma-BHC...	4.335	3.593	298.2E6	83678775	89.901m	55.856m#
4)	MA Heptachlor	4.924	3.933	174.3E6	149.7E6	50.140m	100.125m#
5)	MB Aldrin	5.268	4.214	186.7E6	117.3E6	54.611	77.967m#
6)	B beta-BHC	4.524	3.892	60748433	29262052	39.967m	40.847
7)	B delta-BHC	4.779	4.122	173.2E6	91862997	51.640m	60.187
8)	B Heptachlo...	5.695	4.716	164.3E6	77208676	54.840	54.880
9)	A Endosulfan I	6.082	5.087	147.5E6	62883208	51.788	50.754
10)	B trans-Chl...	5.952	4.967	157.2E6	72567058	51.124	53.665
11)	B cis-Chlor...	6.031	5.030	160.7E6	71126562	50.685	50.415
12)	B 4,4'-DDE	6.204	5.220	300.4E6	139.0E6	103.095	114.975
13)	MA Dieldrin	6.358	5.351	332.6E6	157.6E6	105.421	113.027
14)	MA Endrin	6.588	5.627	272.4E6	125.2E6	105.660	101.268
15)	B Endosulfa...	6.808	5.921	261.9E6	131.1E6	98.493	108.966
16)	A 4,4'-DDD	6.722	5.774	261.4E6	110.9E6	115.674	117.045
17)	MA 4,4'-DDT	7.035	6.025	230.5E6	101.5E6	103.232m	108.357
18)	B Endrin al...	6.938	6.100	157.2E6	70091614	84.095	83.561
19)	B Endosulfa...	7.173	6.323	252.9E6	115.2E6	101.260	103.255
20)	A Methoxychlor	7.513	6.600	612.2E6	240.0E6	462.513	449.809
21)	B Endrin ke...	7.660	6.830	308.2E6	126.7E6	111.323	98.983

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
Data File : PD076810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 10:04
Operator : AR\AJ
Sample : 03418-22MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 13:46:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

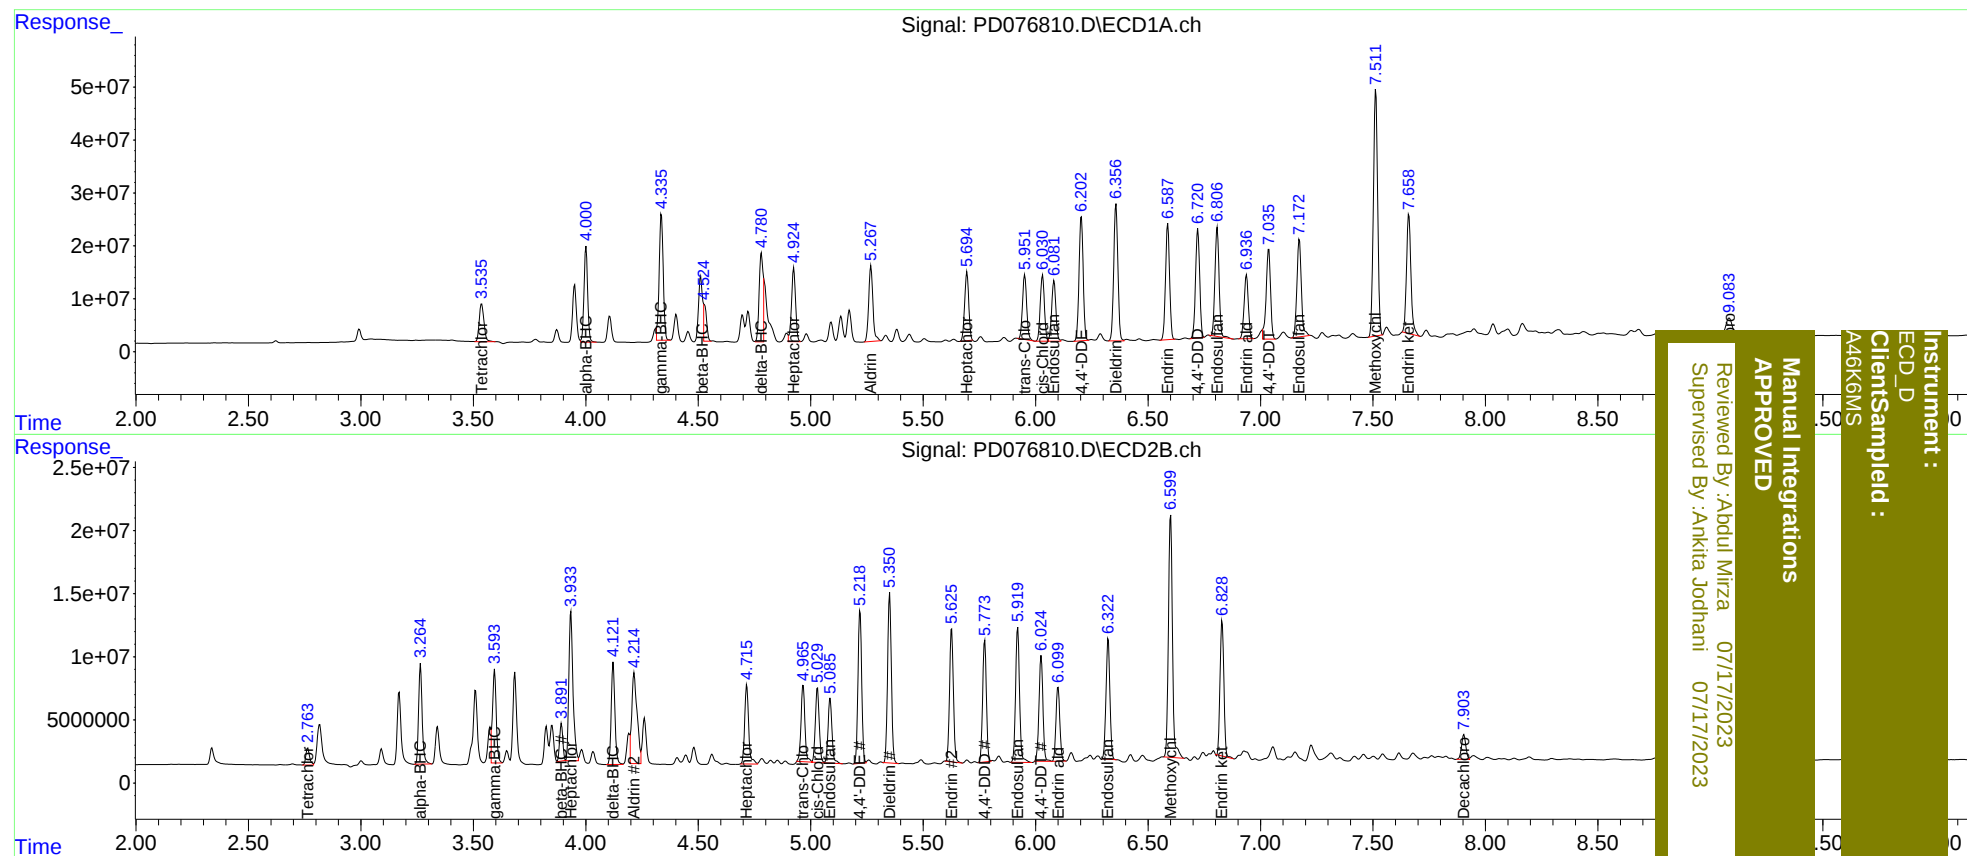

Reviewed By: Abdul Miza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
A46K6MS