

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
 Data File : PD076812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 10:31
 Operator : AR\AJ
 Sample : 03458-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46N1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/17/2023
 Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 13:46:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.763	26271352	9564375	12.349m	8.960m#
2)	SA Decachlor...	9.085	7.904	43008146	19337925	17.703	18.039
Target Compounds							
3)	MA gamma-BHC...	4.337	3.573	2621780	1953589	0.790m	1.304m#
12)	B 4,4'-DDE	6.198	5.218	727775	330766	0.250m	0.274m
14)	MA Endrin	6.583	5.641	984256	609516	0.382m	0.493m#
16)	A 4,4'-DDD	6.725	5.772	1615282	495032	0.715m	0.522m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
Data File : PD076812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 10:31
Operator : AR\AJ
Sample : 03458-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 13:46:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

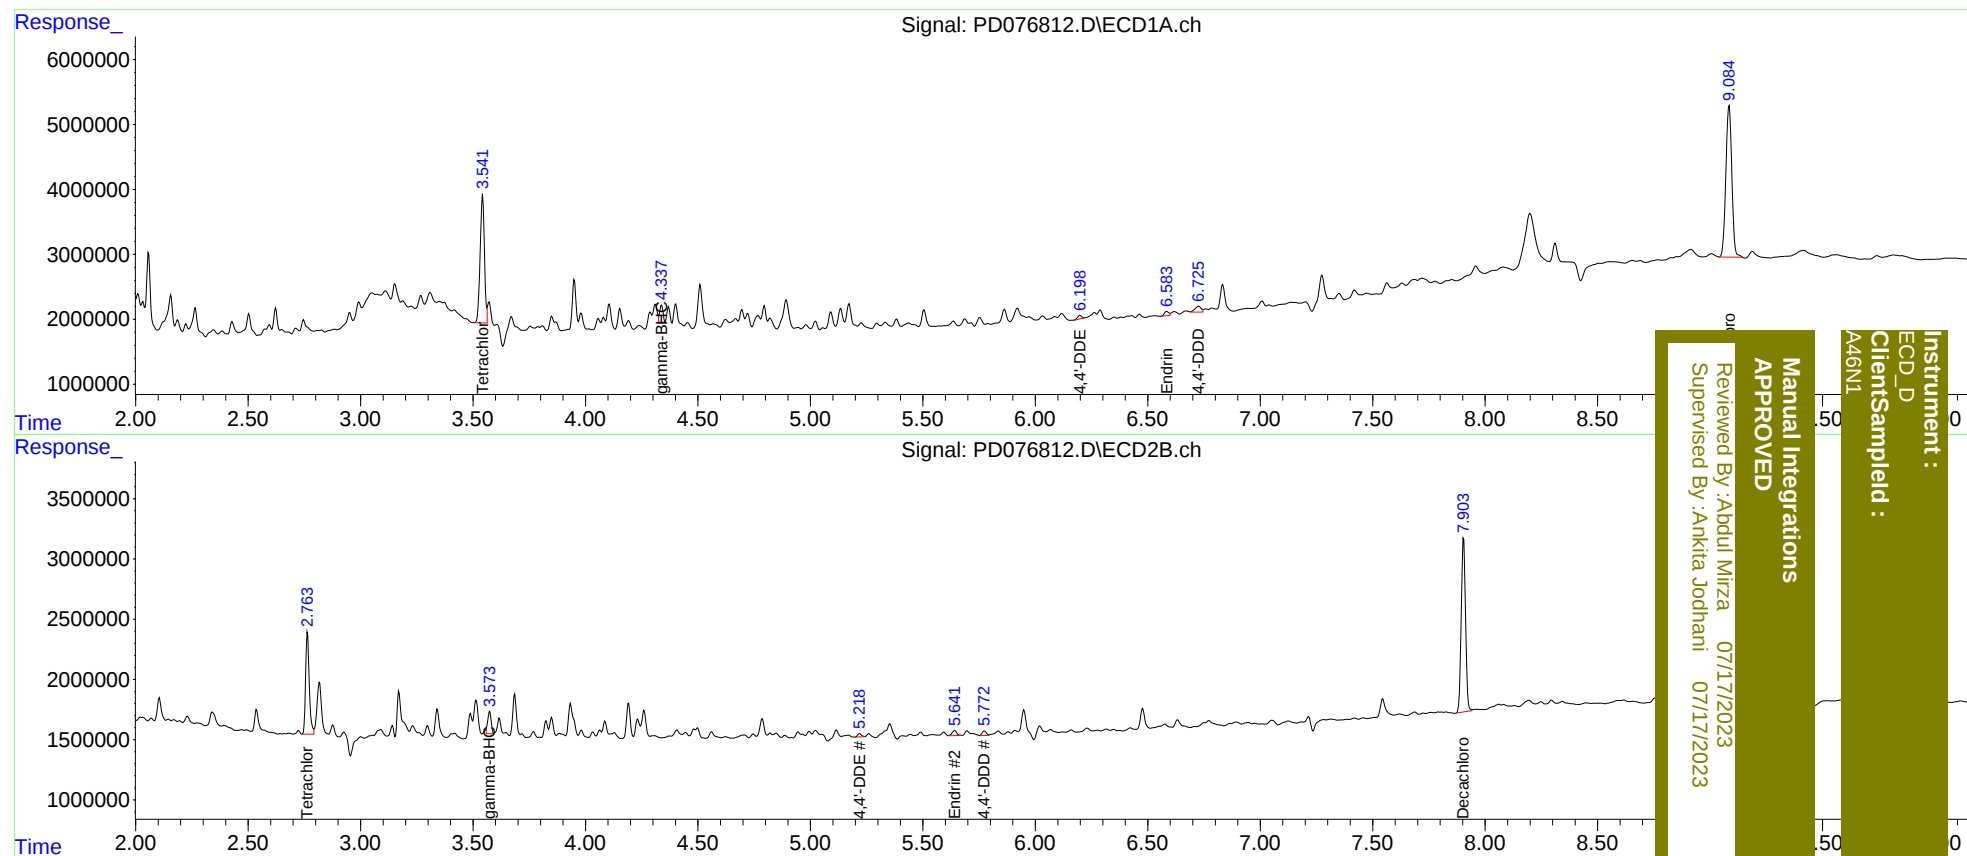

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/17/2023
Supervised By: Ankita Jodhani 07/17/2023

Instrument :
ECD_D
ClientSampled :
A46N1