

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
 Data File : PD076842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 19:18
 Operator : AR\AJ
 Sample : 03472-31MSD
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46Q2MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/19/2023
 Supervised By : Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 13:21:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.765	42965482	17053562	20.197	15.976
2)	SA Decachlor...	9.084	7.904	66762997	30034990	27.480	28.018
Target Compounds							
2)	A alpha-BHC	4.001	3.266	188.7E6	86069516	53.236	54.393
3)	MA gamma-BHC...	4.333	3.594	223.1E6	86048184	67.259m	57.437m
4)	MA Heptachlor	4.925	3.934	171.3E6	104.6E6	49.267	69.977 #
5)	MB Aldrin	5.267	4.214	181.7E6	94119241	53.130	62.539m
6)	B beta-BHC	4.529	3.893	83277850	30819869	54.790m	43.022
7)	B delta-BHC	4.778	4.122	191.9E6	85661939	57.219m	56.124
8)	B Heptachlo...	5.694	4.717	166.8E6	73059329	55.683	51.930
9)	A Endosulfan I	6.081	5.087	145.5E6	66634350	51.100	53.781
10)	B trans-Chl...	5.951	4.967	149.2E6	69959901	48.515	51.737
11)	B cis-Chlor...	6.031	5.031	159.5E6	72108384	50.319	51.111
12)	B 4,4'-DDE	6.203	5.219	311.1E6	136.8E6	106.793	113.182
13)	MA Dieldrin	6.357	5.351	334.1E6	161.3E6	105.871	115.668
14)	MA Endrin	6.587	5.627	285.8E6	134.4E6	110.883	108.726
15)	B Endosulfa...	6.807	5.921	274.1E6	128.7E6	103.078	107.036
16)	A 4,4'-DDD	6.721	5.775	251.9E6	108.0E6	111.502	113.949
17)	MA 4,4'-DDT	7.036	6.026	262.0E6	119.9E6	117.356	128.017
18)	B Endrin al...	6.937	6.100	182.4E6	83286219	97.539	99.291
19)	B Endosulfa...	7.172	6.323	254.2E6	118.1E6	101.797	105.821
20)	A Methoxychlor	7.513	6.599	695.4E6	300.0E6	525.364	562.205m
21)	B Endrin ke...	7.659	6.830	287.8E6	139.3E6	103.942	108.863

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
Data File : PD076842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 19:18
Operator : AR\AJ
Sample : 03472-31MSD
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 13:21:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

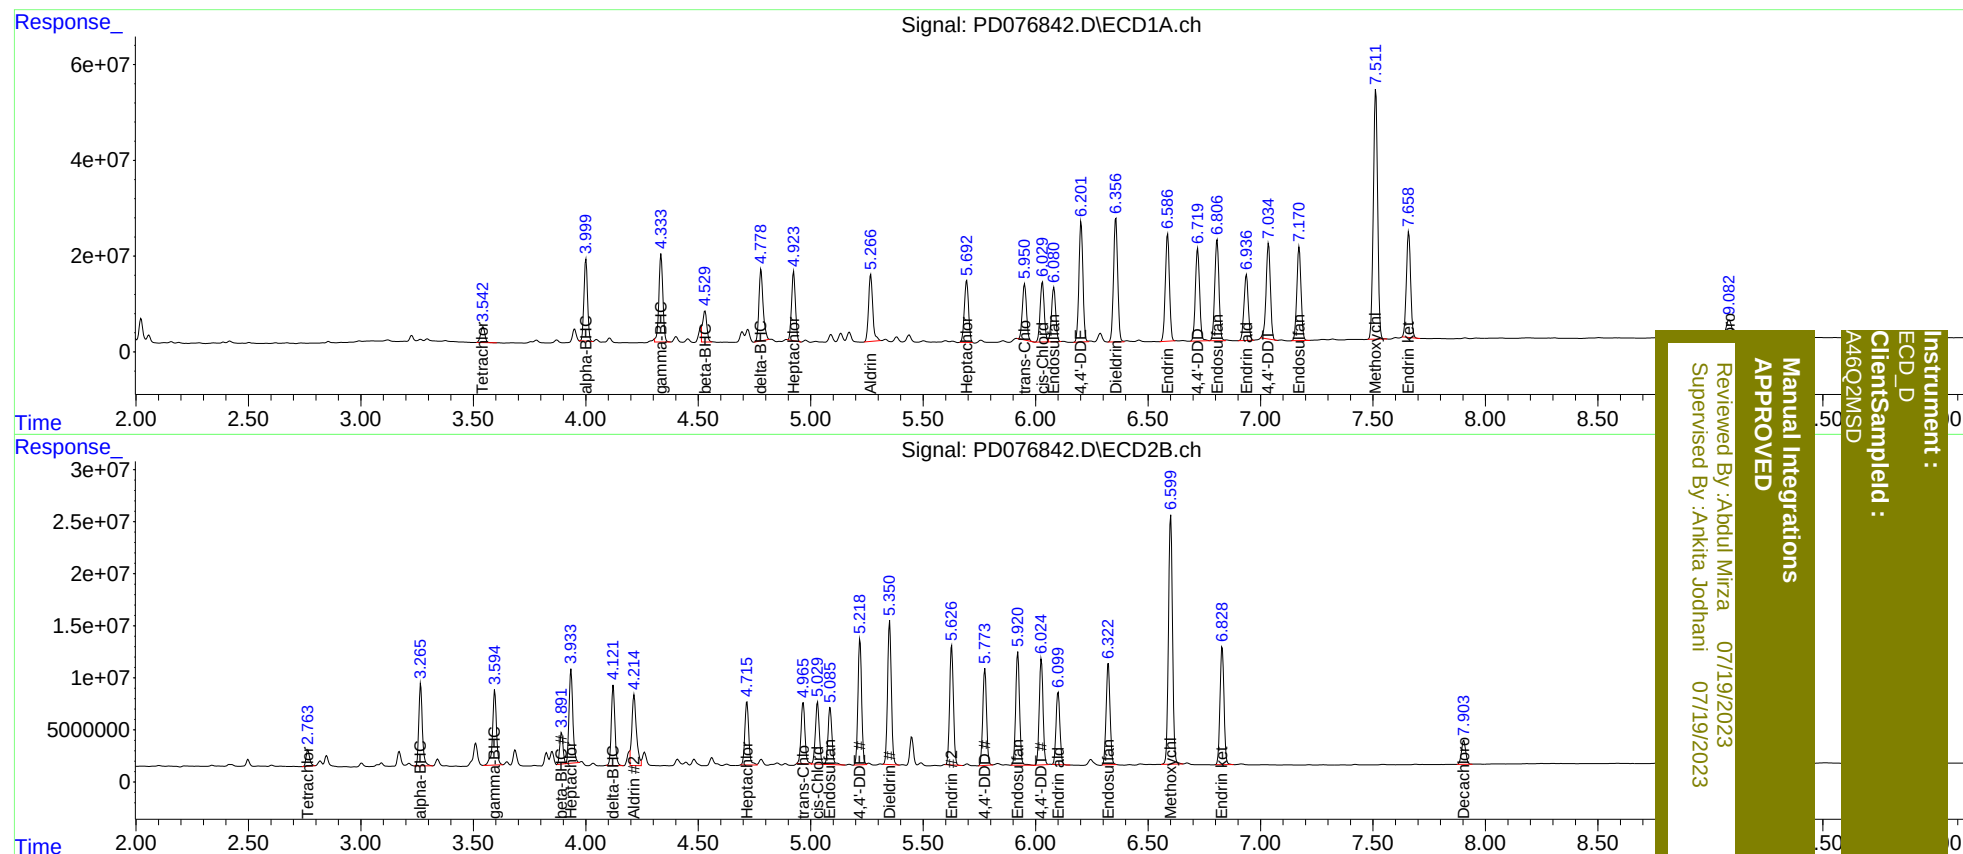

Instrument :
ECD_D
ClientSampled :
A46Q2MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/19/2023
Supervised By: Ankita Jodhani 07/19/2023